

Bidirectional Programmable DC Power Supply

IT6600C Series User Manual



Model: IT6600C

Version: V1.6/2026.4

Notices

© Itech Electronic, Co., Ltd. 2026
No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior permission and written consent from Itech Electronic, Co., Ltd. as governed by international copyright laws.

Manual Part Number

IT6600C

Revision

1st Edition: April 24, 2026.
Itech Electronic, Co., Ltd.

Trademarks

Pentium is U.S. registered trademarks of Intel Corporation.

Microsoft, Visual Studio, Windows and MS Windows are registered trademarks of Microsoft Corporation in the United States and/or other countries and regions.

Warranty

The materials contained in this document are provided “as is”, and is subject to change, without prior notice, in future editions. Further, to the maximum extent permitted by applicable laws, ITECH disclaims all warrants, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. ITECH shall not be held liable for errors or for incidental or indirect damages in connection with the furnishing, use or application of this document or of any information contained herein. Should ITECH and the user enter into a separate written agreement with warranty terms covering the materials in this document that conflict with these terms, the warranty terms in the separate agreement shall prevail.

Technology Licenses

The hardware and/or software described herein are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

Restricted permissions of the U.S. government. Permissions for software and technical data which are authorized to the U.S. Government only include those for custom provision to end users. ITECH provides this customary commercial license in software and technical data pursuant to FAR 12.211 (Technical Data) and 12.212 (Computer Software) and DFARS 252.227-7015 (Technical Data – Commercial Items) and DFARS 227.7202-3 (Rights in Commercial Computer Software or Computer Software Documentation).

Safety Notices

CAUTION

A CAUTION sign denotes a hazard. It calls attention to an operating procedure or practice that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION sign until the indicated conditions are fully understood and met.

WARNING

A WARNING sign denotes a hazard. It calls attention to an operating procedure or practice that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING sign until the indicated conditions are fully understood and met.



NOTE

A NOTE sign denotes important hint. It calls attention to tips or supplementary information that is essential for users to refer to.

Quality Certification and Assurance

We certify that IT6600 series power supply meets all the published specifications at time of shipment from the factory.

Warranty

ITECH warrants that the product will be free from defects in material and workmanship under normal use for a period of one (1) year from the date of delivery (except those described in the Limitation of Warranty below).



Note

Visit <https://www.itechate.com/en/support/register.html> to complete product registration by filling out the necessary information to extend the warranty to two (2) years.

For warranty service or repair, the product must be returned to a service center designated by ITECH.











- The product returned to ITECH for warranty service must be shipped PREPAID. And ITECH will pay for return of the product to customer.
- If the product is returned to ITECH for warranty service from overseas, all the freights, duties and other taxes shall be on the account of customer.




Limitation of Warranty

This Warranty will be rendered invalid if the product is:

- Damaged resulting from customer-wired circuits or customer-supplied parts or accessories;
- Modified or repaired by customer without authorization;
- Damaged resulting from customer-wired circuits or use in an environment not designated by us;
- The product model or serial number is altered, deleted, removed or made illegible by customer;
- Damaged as a result of accidents, including but not limited to lightning, moisture, fire, improper use or negligence.

Safety Symbols

| | | | |
|---|-------------------------------------|---|--------------------|
|  | Direct current |  | ON (power) |
|  | Alternating current |  | OFF (power) |
|  | Both direct and alternating current |  | Power-on state |
|  | Chassis (earth ground) symbol. |  | Power-off state |
|  | Earth (ground) terminal |  | Reference terminal |

| | | | |
|---|---|---|-------------------|
|  | Caution | + | Positive terminal |
|  | Warning (refer to this manual for specific Warning or Caution information) | — | Negative terminal |
|  | A chassis terminal | - | - |

Safety Precautions

The following safety precautions must be observed during all phases of operation of this instrument. Failure to comply with these precautions or specific warnings elsewhere in this manual will constitute a default under safety standards of design, manufacture and intended use of the instrument. ITECH assumes no liability for the customer's failure to comply with these precautions.

WARNING

- Do not use the instrument if it is damaged. Before operation, check the casing to see whether it cracks. Do not operate the instrument in the presence of inflammable gasses, vapors or dusts.
- The instrument is provided with a power cord during delivery and should be connected to a socket with a protective earth terminal, a junction box or a three-phase distribution box. Before operation, be sure that the instrument is well grounded.
- Check all marks on the instrument before connecting the instrument to power supply.
- Use electric wires of appropriate load. All loading wires should be capable of bearing maximum short-circuit of electronic load without overheating. If there are multiple loads, each pair of the load power cord must be carry out the full rated short-circuit output current of the power securely.
- Ensure the voltage fluctuation of mains supply is less than 10% of the working voltage range in order to reduce risks of fire and electric shock.
- Do not install alternative parts on the instrument or perform any unauthorized modification.
- Do not use the instrument if the detachable cover is removed or loosen.
- To prevent the possibility of accidental injuries, be sure to use the power adapter supplied by the manufacturer only.
- We do not accept responsibility for any direct or indirect financial damage or loss of profit that might occur when using the instrument.
- This instrument is used for industrial purposes, do not apply this product to IT power supply system.
- Never use the instrument with a life-support system or any other equipment subject to safety requirements.

WARNING

- **SHOCK HAZARD Ground the Instrument.** This product is provided with a protective earth terminal. To minimize shock hazard, the instrument must be connected to the AC mains through a grounded power cord, with the ground wire firmly connected to an electrical ground (safety ground) at the power outlet or distribution box. Any interruption of the protective (grounding) conductor or disconnection of the protective earth terminal will cause a potential shock hazard that could result in injury or death.
- **Before applying power, verify that all safety precautions are taken.** All connections must be made with the instrument turned off, and must be performed by qualified personnel who are aware of the hazards involved. Improper actions can cause fatal injury as well as equipment damage.
- **SHOCK HAZARD, LETHAL VOLTAGES** This product can input the dangerous voltage that can cause personal injury, and the operator must always be protected from electric shock. Ensure that the input electrodes are either insulated or covered using the safety covers provided, so that no accidental contact with lethal voltages can occur.
- **Never touch cables or connections immediately after turning off the instrument.** Verify that there is no dangerous voltage on the electrodes or sense terminals before touching them.

CAUTION

- Failure to use the instrument as directed by the manufacturer may render its protective features void.
- Always clean the casing with a dry cloth. Do not clean the internals.
- Make sure the vent hole is always unblocked.

Environmental Conditions

The instrument is designed for indoor use and an area with low condensation. The table below shows the general environmental requirements for the instrument.

| Environmental Conditions | Requirements |
|--------------------------|------------------------------|
| Operating temperature | 0°C~50°C |
| Operating humidity | 20%~80%(non-condensation) |
| Storage temperature | -10°C~70 °C |
| Altitude | Operating up to 2,000 meters |
| Installation category | II |
| Pollution degree | Pollution degree 2 |





Note

To make accurate measurements, allow the instrument to warm up for 30 min.

Regulatory Markings



The CE mark indicates that the product complies with all the relevant European legal directives. The specific year (if any) affixed refers to the year when the design was approved.

| | |
|---|--|
|  | <p>The instrument complies with the WEEE Directive (2002/96/EC) marking requirement. This affix product label indicates that you must not discard the electrical/electronic product in domestic household waste.</p> |
|  | <p>This symbol indicates the time period during which no hazardous or toxic substances are expected to leak or deteriorate during normal use. The expected useful life of the product is 10 years. The product can be used safely during the 10-year Environment Friendly Use Period (EFUP). Upon expiration of the EFUP, the product must be immediately recycled.</p> |

Waste Electrical and Electronic Equipment (WEEE) Directive



2002/96/EC Waste Electrical and Electronic Equipment (WEEE) Directive

This product complies with the WEEE Directive (2002/96/EC) marking requirement. This affix product label indicates that you must not discard the electrical/electronic product in domestic household waste.

Product Category

With reference to the equipment classifications described in the Annex 1 of the WEEE Directive, this instrument is classified as a "Monitoring and Control Instrument".

To return this unwanted instrument, contact your nearest ITECH office.



Compliance Information

Complies with the essential requirements of the following applicable European Directives, and carries the CE marking accordingly:

- Electromagnetic Compatibility (EMC) Directive 2014/30/EU
- Low-Voltage Directive (Safety) 2014/35/EU

Conforms with the following product standards:

EMC Standard

IEC 61326-1 / EN 61326-1 ¹²³

Reference Standards

CISPR 11, Class A

IEC 61000-3-2

IEC 61000-3-3

IEC 61000-4-2

IEC 61000-4-3

IEC 61000-4-4

IEC 61000-4-5

IEC 61000-4-6

IEC 61000-4-11

1. The product is intended for use in non-residential/non-domestic environments. Use of the product in residential/domestic environments may cause electromagnetic interference.
2. Connection of the instrument to a test object may produce radiations beyond the specified limit.
3. Use high-performance shielded interface cable to ensure conformity with the EMC standards listed above.

Safety Standard


IEC 61010-1:2010+A1:2016



Note

This section provides general and universal terms. For more detailed information on the Declaration of Conformity, please contact ITECH personnel.

Content

| | |
|--|-----------|
| Quality Certification and Assurance | i |
| Warranty | i |
| Limitation of Warranty | i |
| Safety Symbols | i |
| Safety Precautions..... | ii |
| Environmental Conditions..... | iii |
| Regulatory Markings | iii |
| Waste Electrical and Electronic Equipment (WEEE) Directive | iv |
|  Compliance Information | v |
| Chapter1 Quick Reference | 1 |
| 1.1 Brief Introduction | 1 |
| 1.2 Models and Options | 2 |
| 1.3 Front Panel | 4 |
| 1.4 Keyboard | 6 |
| 1.5 Rear Panel | 8 |
| 1.6 Home-Screen Overview | 12 |
| 1.7 Instrument Installation and Dimensions | 16 |
| Chapter2 Inspection and Installation | 24 |
| 2.1 Unpacking and Transportation | 24 |
| 2.2 Verifying the Shipment..... | 26 |
| 2.3 Connecting the Power Cord | 27 |
| 2.4 Connecting Test Lines (Optional)..... | 29 |
| Chapter3 Getting Started | 33 |
| 3.1 Power-on the Instrument..... | 33 |
| 3.2 Touch Screen Introduction | 34 |
| 3.3 Set output parameters | 35 |
| 3.4 Output On/Off Control..... | 35 |
| Chapter4 Power Supply Function..... | 37 |
| 4.1 Source Mode/ Load Mode Switch | 37 |
| 4.1.1 Source Mode | 37 |
| 4.1.2 Only load mode..... | 38 |
| 4.1.3 Battery simulation mode..... | 38 |
| 4.2 Output Function | 39 |
| 4.2.1 Set the Output Mode..... | 39 |
| 4.2.2 Set the Output Priority Mode..... | 40 |
| 4.2.3 Set Output Slew..... | 42 |
| 4.2.4 Set the Internal Resistance | 43 |
| 4.2.5 Set the Output-On/Output-Off Delay | 44 |
| 4.2.6 Enable the Output..... | 44 |
| 4.3 Protection Function..... | 44 |
| 4.3.1 Over Voltage Protection | 45 |
| 4.3.2 Over Current protection | 45 |
| 4.3.2 Over Power protection | 46 |
| 4.3.4 Under Voltage Protection..... | 46 |
| 4.3.5 Under Current Protection | 47 |
| 4.3.6 Set Maximum Voltage/Current/Power Limit..... | 47 |
| 4.3.7 Over-temperature protection (OTP) | 48 |
| 4.3.8 Sense Reverse Protection | 48 |
| 4.4 LIST Function | 48 |
| 4.4.1 ARB Function | 53 |
| 4.5 Battery Charging/Discharging Test Function | 56 |
| 4.6 Battery Simulation Function..... | 58 |
| 4.7 Built-in Waveform Function | 64 |

| | |
|---|------------|
| 4.7.1 DIN40839 | 64 |
| 4.7.2 ISO16750-2..... | 66 |
| 4.7.3 ISO21848..... | 73 |
| 4.7.4 SAEJ1113-11..... | 75 |
| 4.7.5 LV123..... | 77 |
| 4.7.6 LV124..... | 83 |
| 4.7.7 LV148..... | 92 |
| 4.7.8 ISO21780..... | 103 |
| 4.7.9 ISO21498-2..... | 115 |
| 4.8 Standard IEC Regulations | 125 |
| 4.8.1 IEC 61000-4-17..... | 126 |
| 4.8.2 IEC 61000-4-29..... | 128 |
| 4.9 Solar Photovoltaic Curve Simulation Function (SAS)..... | 129 |
| Chapter5 System-Related Functions | 135 |
| 5.1 System Menu Reference | 135 |
| 5.2 Configuration Menu Reference..... | 139 |
| 5.3 Key Lock Function..... | 140 |
| 5.4 Switching Local/Remote Mode | 140 |
| 5.5 Save and Recall Operations | 140 |
| 5.6 Screen Capture Function..... | 141 |
| 5.7 Query the System Log | 141 |
| 5.8 Multi-units operation | 141 |
| 5.8.1 Series Operation(single-unit) | 141 |
| 5.8.2 Parallel Operation(single-unit)..... | 143 |
| 5.8.3 Parallel Operation(multi-masters) | 144 |
| 5.8.4 Parallel Operation(one master and multi-slaves) | 149 |
| 5.8.5 Parallel Operation(cabinet model)..... | 152 |
| 5.9 Digital I/O Function | 156 |
| 5.9.1 Description of Digital I/O pin..... | 156 |
| 5.9.2 I/O Control | 159 |
| 5.10 Analogue Function (Ext-Program) (Optional)..... | 162 |
| 5.11 Redundant function | 166 |
| Chapter6 Measurement Functions..... | 169 |
| 6.1 Meter Mode | 169 |
| 6.2 Oscilloscope Mode | 170 |
| 6.3 Recorder Function | 173 |
| 6.4 Query the Energy | 175 |
| Chapter7 Technical Specifications | 176 |
| 7.1 Supplemental characteristics | 176 |
| 7.2 Main technical parameters | 176 |
| IT6642C-1200-200..... | 176 |
| IT6684C-1200-400..... | 178 |
| IT66126C-1200-600..... | 180 |
| IT66168C-1200-800..... | 182 |
| IT66210C-1200-1000..... | 184 |
| IT66252C-1200-1200..... | 186 |
| IT66294C-1200-1400..... | 188 |
| IT66336C-1200-1600..... | 190 |
| IT66378C-1200-1800..... | 193 |
| IT66420C-1200-2000..... | 195 |
| IT6642C-1600-140..... | 197 |
| IT6684C-1600-280..... | 199 |
| IT66126C-1600-420..... | 201 |
| IT66168C-1600-560..... | 203 |
| IT66210C-1600-700..... | 205 |
| IT66252C-1600-840..... | 207 |
| IT66294C-1600-980..... | 209 |

| | |
|--|------------|
| <i>IT66336C-1600-1120</i> | 211 |
| <i>IT66378C-1600-1260</i> | 213 |
| <i>IT66420C-1600-1400</i> | 215 |
| <i>IT6642C-2250-100</i> | 218 |
| <i>IT6684C-2250-200</i> | 220 |
| <i>IT66126C-2250-300</i> | 222 |
| <i>IT66168C-2250-400</i> | 224 |
| <i>IT66210C-2250-500</i> | 226 |
| <i>IT66252C-2250-600</i> | 228 |
| <i>IT66294C-2250-700</i> | 230 |
| <i>IT66336C-2250-800</i> | 232 |
| <i>IT66378C-2250-900</i> | 234 |
| <i>IT66420C-2250-1000</i> | 236 |
| Chapter8 Remote Control | 239 |
| 8.1 USB Interface..... | 239 |
| 8.2 LAN Interface..... | 239 |
| 8.2.1 Using Web Server | 240 |
| 8.2.2 Using Telnet..... | 241 |
| 8.2.3 Using Sockets | 242 |
| 8.2.4 Using VNC | 242 |
| 8.3 CAN Interface | 244 |
| 8.4 GPIB Interface (Optional) | 245 |
| 8.5 RS232 Interface (Optional) | 246 |
| 8.6 EtherCAT Interface (Optional) | 248 |
| Appendix | 249 |
| Specifications of Red and Black Test Lines | 249 |

Chapter1 Quick Reference

This chapter briefly introduces the front panel, rear panel, keyboard and screen display of the product, which provides you with a quick overview of its appearance, structure and key functions before operating. This chapter will not specify each operation in detail, it is just a guide to get you started quickly.

1.1 Brief Introduction

IT6600C series DC power supply is a new generation graphical bidirectional DC power supply. It adopts a touch screen design and intuitive GUI, making parameter setting and waveform editing simpler and more efficient. It adopts advanced third-generation SiC technology. A 3U height single unit can output 21kW each in dual channels. If the two independent channels are connected in series/parallel, it can reach maximum power 42kW. Since 1 unit IT6600C can cover the output range of 3-5 normal power supplies, it can be applied to various applications requiring high voltage or high current.

IT6600C series is not only a power supply, but also an excellent electronic load. It can not only output power as a DC power supply, but also act as a DC electronic load, absorbing power and feeding clean power back to the grid to realize energy recycling. IT6600C series brings you a new experience during the high-power complex testing in the fields of automobiles, energy storage, industry, green energy and so on and provides strong support for R&D, verification, production, etc.

Features

- Bidirectional, integrating power supply and e-load in one.
- High power density, up to 42kW in 3U.
- Independent dual-channel design in 3U unit, and channels can be connected in series or parallel.
- High efficient power regeneration.
- Master-slave current sharing, output max. 10MW in parallel.
- 5-inch touch screen with intuitive GUI.
- Dynamic response $\leq 200\mu s$
- Rise time $\leq 1ms$
- High precision $\leq 0.03\% + 30mA$
- Built-in communication interface: USB/LAN/CAN 2.0B/Digital IO.
- Optional communication interface: GPIB/EtherCAT/Analog&RS232.
- Built-in standard multi-channel solar array simulation software (SAS1000MD).
- List function, dynamic working condition simulation with tens of millions of points.
- Built-in IEC 61000-4-17/IEC 61000-4-29 waveforms. *1
- Built-in 9 standard automotive voltage curves, including LV123, LV148, ISO21498-2, etc.

*1. IT6600C can partially meet test requirements of IEC61000-4-17.

1.2 Models and Options

This series models include:

- One master and multi-slaves series

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|--------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT6642C-1200-200 | 600V/±100A/±21kW*2ch | 600V/±200A/±42kW*1ch | 1200V/±100A/±42kW*1ch | 3U |
| IT6684C-1200-400 | 600V/±200A/±42kW*2ch | 600V/±400A/±84kW*1ch | 1200V/±200A/±84kW*1ch | 15U |
| IT66126C-1200-600 | 600V/±300A/±63kW*2ch | 600V/±600A/±126kW*1ch | 1200V/±300A/±126kW*1ch | 15U |
| IT66168C-1200-800 | 600V/±400A/±84kW*2ch | 600V/±800A/±168kW*1ch | 1200V/±400A/±168kW*1ch | 27U |
| IT66210C-1200-1000 | 600V/±500A/±105kW*2ch | 600V/±1000A/±210kW*1ch | 1200V/±500A/±210kW*1ch | 27U |
| IT66252C-1200-1200 | 600V/±600A/±126kW*2ch | 600V/±1200A/±252kW*1ch | 1200V/±600A/±252kW*1ch | 27U |
| IT66294C-1200-1400 | 600V/±700A/±147kW*2ch | 600V/±1400A/±294kW*1ch | 1200V/±700A/±294kW*1ch | 27U |
| IT66336C-1200-1600 | 600V/±800A/±168kW*2ch | 600V/±1600A/±336kW*1ch | 1200V/±800A/±336kW*1ch | 37U |
| IT66378C-1200-1800 | 600V/±900A/±189kW*2ch | 600V/±1800A/±378kW*1ch | 1200V/±900A/±378kW*1ch | 37U |
| IT66420C-1200-2000 | 600V/±1000A/±210kW*2ch | 600V/±2000A/±420kW*1ch | 1200V/±1000A/±420kW*1ch | 37U |

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|--------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT6642C-1600-140 | 800V/±70A/±21kW*2ch | 800V/±140A/±42kW*1ch | 1600V/±70A/±42kW*1ch | 3U |
| IT6684C-1600-280 | 800V/±140A/±42kW*2ch | 800V/±280A/±84kW*1ch | 1600V/±140A/±84kW*1ch | 15U |
| IT66126C-1600-420 | 800V/±210A/±63kW*2ch | 800V/±420A/±126kW*1ch | 1600V/±210A/±126kW*1ch | 15U |
| IT66168C-1600-560 | 800V/±280A/±84kW*2ch | 800V/±560A/±168kW*1ch | 1600V/±280A/±168kW*1ch | 27U |
| IT66210C-1600-700 | 800V/±350A/±105kW*2ch | 800V/±700A/±210kW*1ch | 1600V/±350A/±210kW*1ch | 27U |
| IT66252C-1600-840 | 800V/±420A/±126kW*2ch | 800V/±840A/±252kW*1ch | 1600V/±420A/±252kW*1ch | 27U |
| IT66294C-1600-980 | 800V/±490A/±147kW*2ch | 800V/±980A/±294kW*1ch | 1600V/±490A/±294kW*1ch | 27U |
| IT66336C-1600-1120 | 800V/±560A/±168kW*2ch | 800V/±1120A/±336kW*1ch | 1600V/±560A/±336kW*1ch | 37U |
| IT66378C-1600-1260 | 800V/±630A/±189kW*2ch | 800V/±1260A/±378kW*1ch | 1600V/±630A/±378kW*1ch | 37U |
| IT66420C-1600-1400 | 800V/±700A/±210kW*2ch | 800V/±1400A/±420kW*1ch | 1600V/±700A/±420kW*1ch | 37U |

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|-------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT6642C-2250-100 | 1200V/±50A/±21kW*2ch | 1200V/±100A/±42kW*1ch | 2250V/±50A/±42kW*1ch | 3U |
| IT6684C-2250-200 | 1200V/±100A/±42kW*2ch | 1200V/±200A/±84kW*1ch | 2250V/±100A/±84kW*1ch | 15U |
| IT66126C-2250-300 | 1200V/±150A/±63kW*2ch | 1200V/±300A/±126kW*1ch | 2250V/±150A/±126kW*1ch | 15U |
| IT66168C-2250-400 | 1200V/±200A/±84kW*2ch | 1200V/±400A/±168kW*1ch | 2250V/±200A/±168kW*1ch | 27U |
| IT66210C-2250-500 | 1200V/±250A/±105kW*2ch | 1200V/±500A/±210kW*1ch | 2250V/±250A/±210kW*1ch | 27U |
| IT66252C-2250-600 | 1200V/±300A/±126kW*2ch | 1200V/±600A/±252kW*1ch | 2250V/±300A/±252kW*1ch | 27U |
| IT66294C-2250-700 | 1200V/±350A/±147kW*2ch | 1200V/±700A/±294kW*1ch | 2250V/±350A/±294kW*1ch | 27U |

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|--------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT66336C-2250-800 | 1200V/±400A/±168kW*2ch | 1200V/±800A/±336kW*1ch | 2250V/±400A/±336kW*1ch | 37U |
| IT66378C-2250-900 | 1200V/±450A/±189kW*2ch | 1200V/±900A/±378kW*1ch | 2250V/±450A/±378kW*1ch | 37U |
| IT66420C-2250-1000 | 1200V/±500A/±210kW*2ch | 1200V/ ± 1000A/ ± 420kW*1ch | 2250V/±500A/±420kW*1ch | 37U |

● Multi-masters series

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|---------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT6684CM-1200-400 | 600V/±200A/±42kW*2ch | 600V/±400A/±84kW*1ch | 1200V/±200A/±84kW*1ch | 15U |
| IT66126CM-1200-600 | 600V/±300A/±63kW*2ch | 600V/±600A/±126kW*1ch | 1200V/±300A/±126kW*1ch | 15U |
| IT66168CM-1200-800 | 600V/±400A/±84kW*2ch | 600V/±800A/±168kW*1ch | 1200V/±400A/±168kW*1ch | 27U |
| IT66210CM-1200-1000 | 600V/±500A/±105kW*2ch | 600V/±1000A/±210kW*1ch | 1200V/±500A/±210kW*1ch | 27U |
| IT66252CM-1200-1200 | 600V/±600A/±126kW*2ch | 600V/±1200A/±252kW*1ch | 1200V/±600A/±252kW*1ch | 27U |
| IT66294CM-1200-1400 | 600V/±700A/±147kW*2ch | 600V/±1400A/±294kW*1ch | 1200V/±700A/±294kW*1ch | 37U |
| IT66336CM-1200-1600 | 600V/±800A/±168kW*2ch | 600V/±1600A/±336kW*1ch | 1200V/±800A/±336kW*1ch | 37U |
| IT66378CM-1200-1800 | 600V/±900A/±189kW*2ch | 600V/±1800A/±378kW*1ch | 1200V/±900A/±378kW*1ch | 37U |

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|---------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT6684CM-1600-280 | 800V/±140A/±42kW*2ch | 800V/±280A/±84kW*1ch | 1600V/±140A/±84kW*1ch | 15U |
| IT66126CM-1600-420 | 800V/±210A/±63kW*2ch | 800V/±420A/±126kW*1ch | 1600V/±210A/±126kW*1ch | 15U |
| IT66168CM-1600-560 | 800V/±280A/±84kW*2ch | 800V/±560A/±168kW*1ch | 1600V/±280A/±168kW*1ch | 27U |
| IT66210CM-1600-700 | 800V/±350A/±105kW*2ch | 800V/±700A/±210kW*1ch | 1600V/±350A/±210kW*1ch | 27U |
| IT66252CM-1600-840 | 800V/±420A/±126kW*2ch | 800V/±840A/±252kW*1ch | 1600V/±420A/±252kW*1ch | 27U |
| IT66294CM-1600-980 | 800V/±490A/±147kW*2ch | 800V/±980A/±294kW*1ch | 1600V/±490A/±294kW*1ch | 37U |
| IT66336CM-1600-1120 | 800V/±560A/±168kW*2ch | 800V/±1120A/±336kW*1ch | 1600V/±560A/±336kW*1ch | 37U |
| IT66378CM-1600-1260 | 800V/±630A/±189kW*2ch | 800V/±1260A/±378kW*1ch | 1600V/±630A/±378kW*1ch | 37U |

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|--------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT6684CM-2250-200 | 1200V/±100A/±42kW*2ch | 1200V/±200A/±84kW*1ch | 2250V/±100A/±84kW*1ch | 15U |
| IT66126CM-2250-300 | 1200V/±150A/±63kW*2ch | 1200V/±300A/±126kW*1ch | 2250V/±150A/±126kW*1ch | 15U |
| IT66168CM-2250-400 | 1200V/±200A/±84kW*2ch | 1200V/±400A/±168kW*1ch | 2250V/±200A/±168kW*1ch | 27U |
| IT66210CM-2250-500 | 1200V/±250A/±105kW*2ch | 1200V/±500A/±210kW*1ch | 2250V/±250A/±210kW*1ch | 27U |
| IT66252CM-2250-600 | 1200V/±300A/±126kW*2ch | 1200V/±600A/±252kW*1ch | 2250V/±300A/±252kW*1ch | 27U |
| IT66294CM-2250-700 | 1200V/±350A/±147kW*2ch | 1200V/±700A/±294kW*1ch | 2250V/±350A/±294kW*1ch | 37U |

| Model | Dual-channel output specifications | Parallel output specifications | Series Output Specifications | Height |
|--------------------|------------------------------------|--------------------------------|------------------------------|--------|
| IT66336CM-2250-800 | 1200V/±400A/±168kW*2ch | 1200V/±800A/±336kW*1ch | 2250V/±400A/±336kW*1ch | 37U |
| IT66378CM-2250-900 | 1200V/±450A/±189kW*2ch | 1200V/±900A/±378kW*1ch | 2250V/±450A/±378kW*1ch | 37U |

Optional accessories


The following optional accessories from ITECH are sold separately. Users need to purchase separately.

| Device Name | Model | Description |
|--------------------------------|----------------|---|
| GPIB communication interface | IT-E176 | When the user needs to use GPIB interface to enable remote operation, this option is the right choice. |
| RS232+Analog | IT-E177 | Interface card that includes RS232 communication interface and external analog. When the user needs to use RS232 or external analog interface to enable remote operation, this option is the right choice. |
| EtherCAT | IT-E1601-black | - |
| Fiber optic modules and cables | IT-E168 | Used for parallel connection between the units in a cabinet, including one fiber module and two fiber cables, with lengths of 1.5 meters and 0.3 meters. The fiber optic module and cable are the necessary accessories for the parallel connection. Different numbers of fiber optic modules and cables are used in different numbers of parallels. |
| Fiber optic modules and cables | IT-E169 | Used for parallel connection between cabinets, including one fiber module and one 2.5m fiber cable. The fiber optic module and cable are the necessary accessories for the parallel connection. Different numbers of fiber optic modules and cables are used in different numbers of parallels. |
| Relay board | IT-E179 | - |
| Series and parallel boxes | IT-E183 | Cabinet configuration, direct switching between series and parallel. |

1.3 Front Panel

- **One master and multi-slaves series**


All of this series instruments have the same front panel. The front panel diagram and key diagram of 3U model is shown in the figure below; descriptions of the numbered items follow the figure.

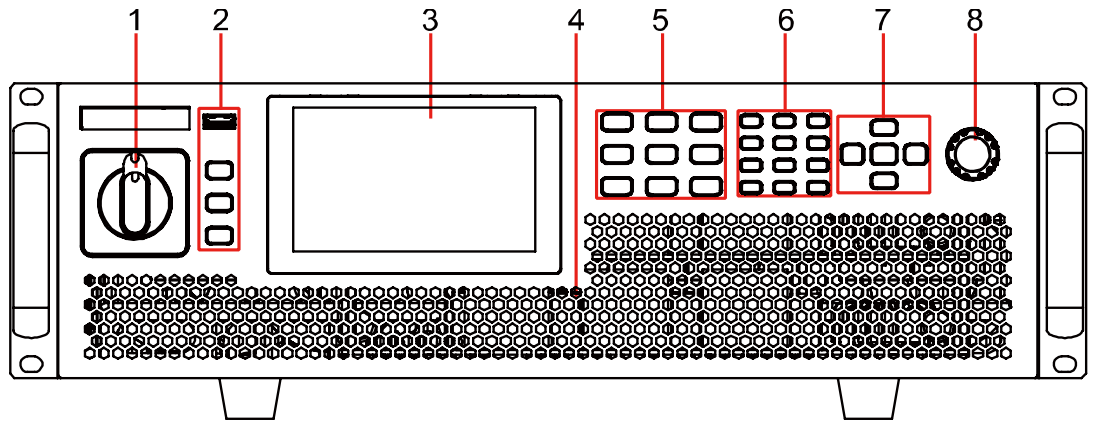


- | | |
|--|----------------------------------|
| 1 Power Switch | 2 USB interface /Print/View/Menu |
| 3 LCD touch screen | 4 Vent hole |
| 5 Function key | 6 Number key |
| 7 Up, down, left and right key and enter key | 8 Rotary knob |

● **Multi-masters series**

The front panel buttons of this series of instruments are the same; the differences lie in the output power or the cabinet size. Below are the front panel diagram and button function diagram for the 27U model.

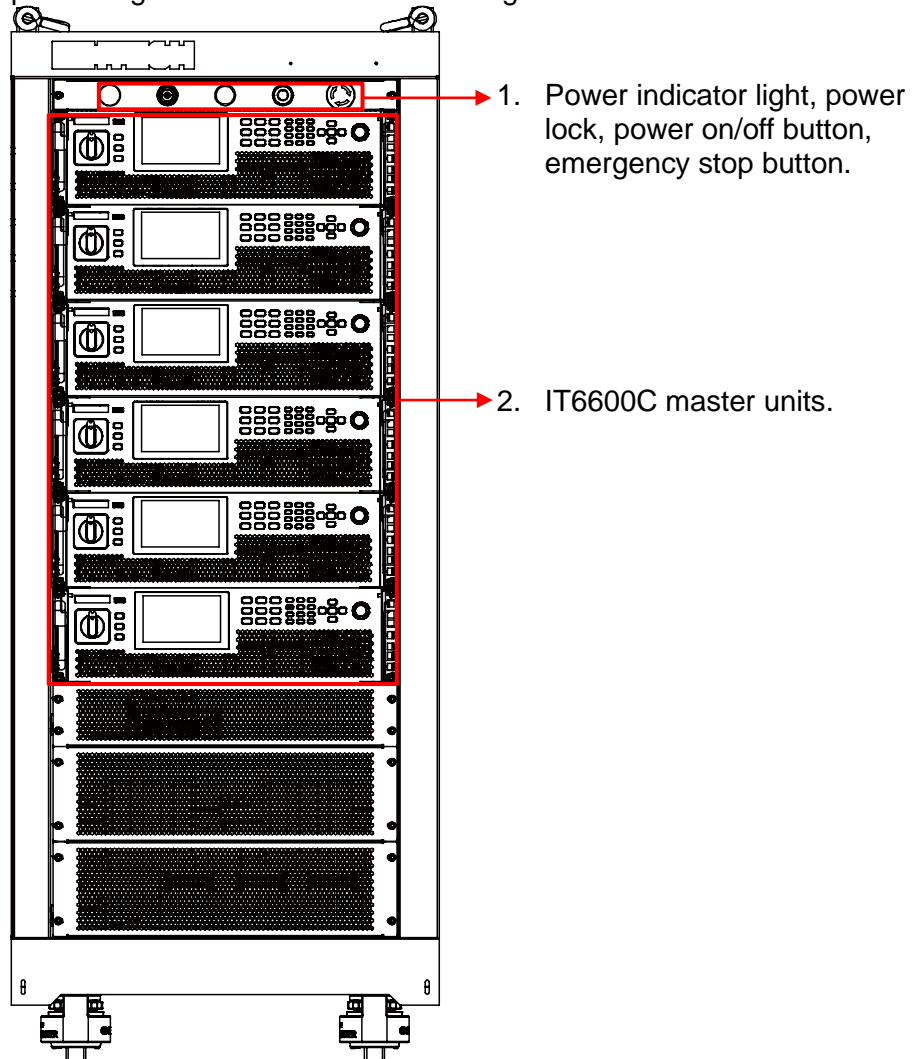


1. Power indicator light, power lock, power on/off button, emergency stop button.

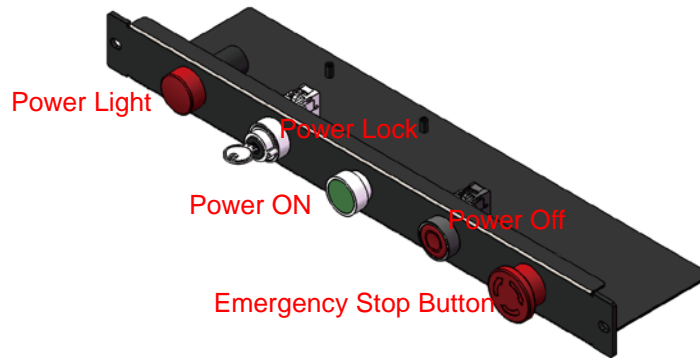

Detailed function description is shown below:

- Power light: When the power switch is pressed, the power light is lighted on.
- After the power lock is activated, press the green power on button to power up the cabinet; when the power lock is deactivated, the green power on button is disabled, preventing the cabinet from powering up.
- The power on button is a green button; pressing the power on button will power up the cabinet.
- The power off button is a red button; pressing the power off button will power down the cabinet.
- The emergency stop button is a rotary resetting button. When the emergency stop button is pressed, the cabinet is powered off; after rotary resetting, the cabinet is powered on.


2. IT6600C master units.

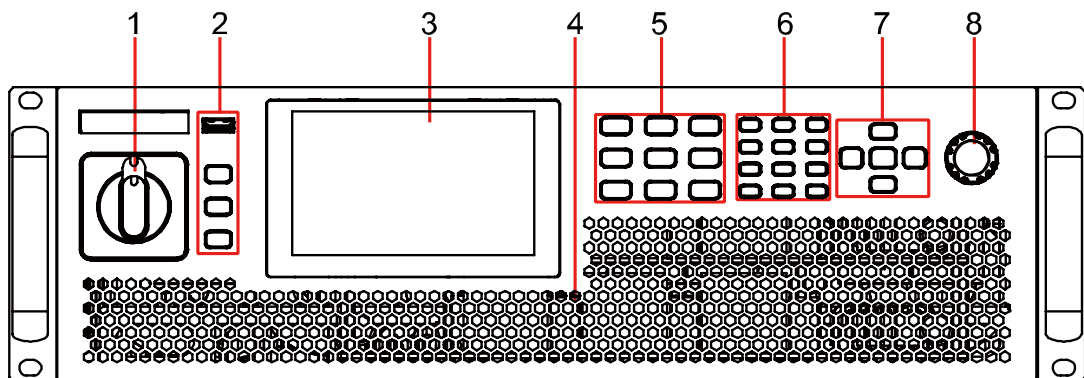

- | | |
|--|----------------------------------|
| 1 Power Switch | 2 USB interface /Print/View/Menu |
| 3 LCD touch screen | 4 Vent hole |
| 5 Function key | 6 Number key |
| 7 Up, down, left and right key and enter key | 8 Rotary knob |

1.4 Keyboard

The keyboard introduction of IT6600 series Power Supply is shown as follows.

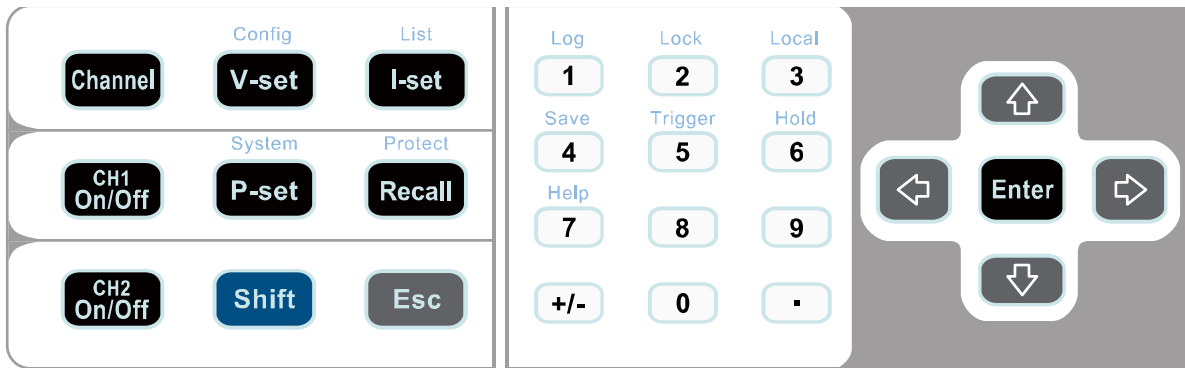

| Keys | Description |
|---------------------------------|---|
| Power | Power Switch |
| Print | Used for saving screen images. |
| View | Interface display switch key. <ul style="list-style-type: none"> In Normal working mode, use this key to switch between the Meter interface, Scope interface, and Recorder interface. In non-Normal working mode, use this key to switch between the function interface, Scope interface, and Recorder interface. |
| Menu | Used for going back to menu page. |
| [Channel] | Switch channels. |
| [V-set] | Set the output voltage value. |
| [I-set] | Set the output current value. |
| [P-set] | Set the output power value. |
| [Recall] | Returns the instrument to the specified setup. |
| [Shift] | Composite key, combined with other keys to realize functions marked above keys. |
| [Esc] | Press this key to exit the current operation interface. |
| CH1 On/Off | Turn the CH1 output on or off. |
| CH2 On/Off | Turn the CH2 output on or off. |
| [0]-[9] | Number key. Enter the number directly. |
| +/- | Positive and negative signs. |
| . | Decimal point. |
| Left / Right Navigation keys | The left and right navigation keys are used to adjust the cursor to the specified position or scrolls pages to view menu items. |
| Up / Down Navigation keys | The up and down navigation keys are used to scroll page up and down to view menu items. |
| [Enter] | Operation confirmation key |

Composite key **[Shift]**, combined with other keys to realize functions marked above keys. Firstly, press **[shift]** and the shift key will be lighted, and then press the function key, the detailed functions are listed as follows.

| Keys | Description |
|---------------------------------|-------------------------------|
| [Shift]+[V-set] (Config) | Enter to Configuration menu. |
| [Shift]+[I-set] (List) | Enter the List function menu. |
| [Shift]+[P-set] (System) | Enter the System menu. |

| Keys | Description |
|---------------------------|---|
| [Shift]+[Recall](Protect) | Enter the Protect menu of the power supply. |
| [Shift]+[1](Log) | Enter the Log query interface. |
| [Shift]+ [2] (Lock) | Turn the keyboard lock on or off. |
| [Shift]+[3] (Local) | Switch remote control mode to local control mode. |
| [Shift]+[4] (Save) | Save the common parameter settings. |
| [Shift]+ [5] (Trigger) | Used for manual trigger. |
| [Shift]+ [6] (Hold) | When you need to keep the present meter status, you can press the keys. Then the present meter status display and will be kept no matter whether output is running. |
| [Shift]+ [7] (Help) | Obtain the help information. |

Push-on Knob

The IT6600 series Power Supply provides a knob on the front panel as shown in the next figure.



The functions of the push-on knob is described as follows.

- Adjust the value setting.
- Select menu item.
- Confirm the set value or the selected menu item.

Adjust the Value Setting

In the value setting interface, rotate the knob clockwise to increase the set value and anticlockwise to decrease the set value.

Select Menu Item

The knob can also be used to view menu items. In the menu item display interface, turning the knob clockwise indicates that the next menu item is selected, and turning the knob anticlockwise indicates that the previous menu item is selected.


Confirm settings

After completing the value setting or selecting a menu item, pushing the knob acts like pressing **[Enter]** key to confirm the operation.

1.5 Rear Panel

- **One master and multi-slaves series**


The rear panel of the IT6600 series 3U model is shown below.

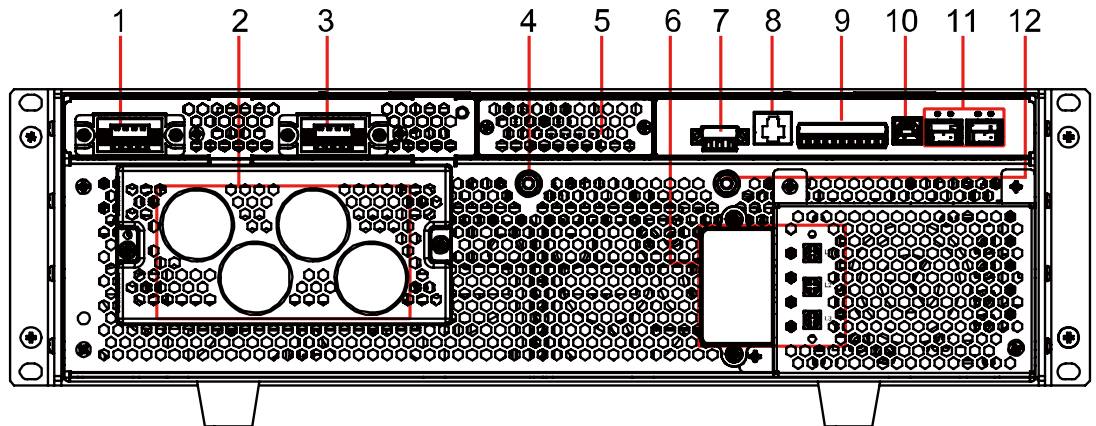

| No. | Name | Description |
|-----|---------------------------------|--|
| 1 | Remote sense Terminals (CH1) | VS1- and VS1+ are remote sense terminals, used for maximizing measurement accuracy. |
| 2 | DC output terminals | Used to connect DUT. (Hole size M8) |
| 3 | Remote sense Terminals (CH2) | VS2- and VS2+ are remote sense terminals, used for maximizing measurement accuracy. |
| 4 | Ground screw | Grounding terminal for connecting the ground of other devices. |
| 5 | Optional expansion slot | Optional interfaces: (Plastic plugs are inserted by default when the user does not purchase the interface.) The optional interface as follows: <ul style="list-style-type: none"> ● GPIB ● RS232/ Analog interface ● EtherCAT ● Relay board |
| 6 | AC power input socket | Used to connect AC power to start instrument. |
| 7 | External control interface CTRL | This interface is used for the parallel connection between the master (with operation panel) and the slaves (without operation panel). Connect the interface on the rear panel of each unit to be connected in parallel, and the master can offer synchronous control over the power-on/off of the slaves. |
| 8 | LAN interface | LAN communication interface. |
| 9 | I/O terminals/CAN interface | <ul style="list-style-type: none"> ● Digital Port ● CAN communication interface CAN-H and CAN-L |
| 10 | USB interface | USB communication interface. |

| | | |
|----|--------------|--|
| 11 | System Bus | Used for communication between instruments in parallel operation feature. <ul style="list-style-type: none"> ● F-TX/F-RX: This interface is used for the parallel connection between the master (with operation panel) and the slaves (without operation panel) for realizing communication of units in parallel. ● TX/RX: This interface is used for the parallel connection between the masters (with operation panel) for the communication of units in parallel. |
| 12 | Ground screw | Protective grounding terminal for AC input. |


Schematic Diagram of Rear Panel of this series (15U) instrument is shown as below, model 27U and model 37U have the same rear panels as 15U model. Only the sizes are different.

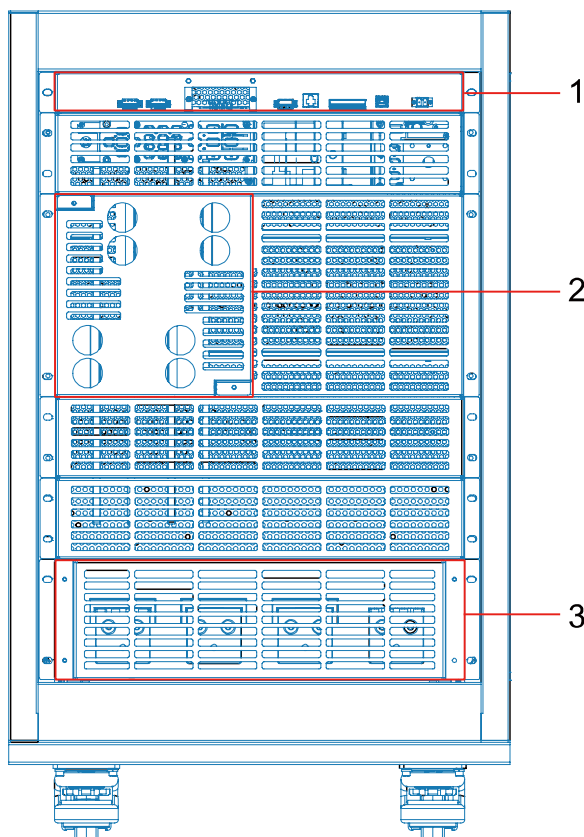

1. The communication interface for cabinet, the detailed diagram as follows, and the descriptions are the same as 3U model.




2. Output terminals (Hole size M8) and protective cover.
3. Input terminal (Hole size M8), connected to the instrument's power supply.

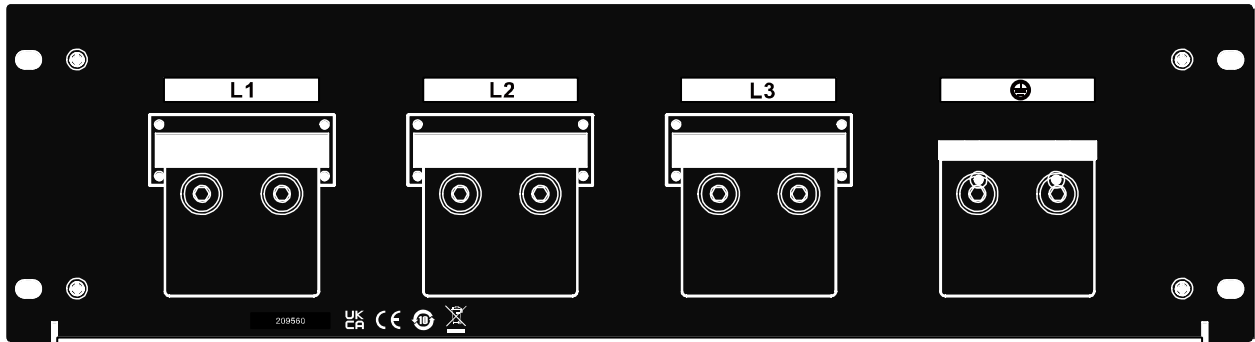


- **Multi-masters series**

Except for the size differences, the rear panel terminals of this series of instruments are completely identical. The following introduction uses the 27U cabinet as an example.

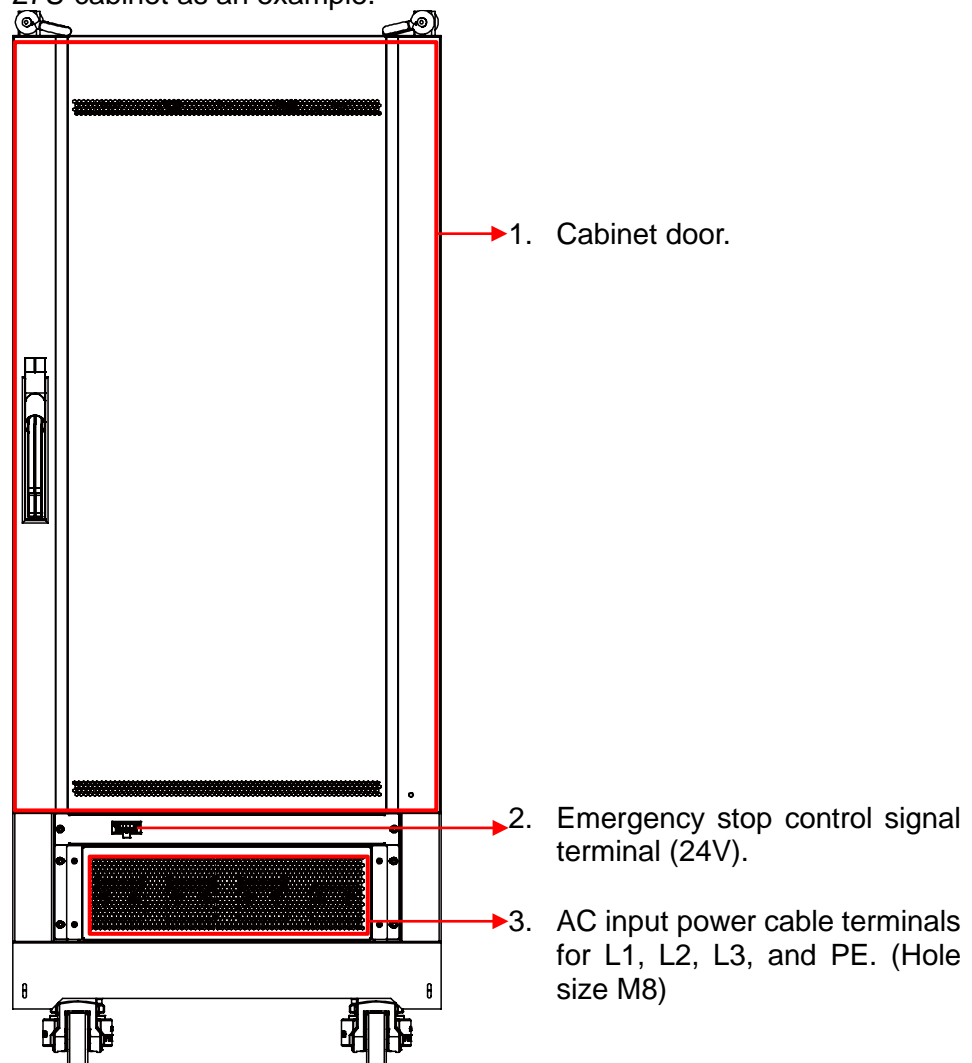

1. Cabinet door. (Make sure the cabinet door is securely closed before powering on.)
2. Emergency stop control signal terminal (24V).
Pin2 and Pin3 of the terminal are shorted by default, as shown in the figure below.

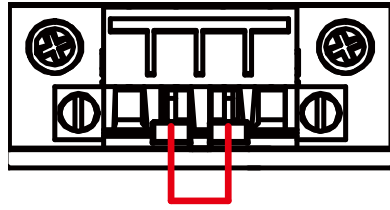


When the cabinet is powered on and off by the emergency stop button on the front panel of the cabinet, make sure that the short-circuit clips here are correctly installed.

When controlling the power on and off of the cabinet (emergency stop) through external cables, refer to the following steps:

- a. Remove the short-circuit clip between Pin2 and Pin3.

Note: Lead 24V voltage signal.

- b. Refer to the figure below to connect to the external signal control circuit.

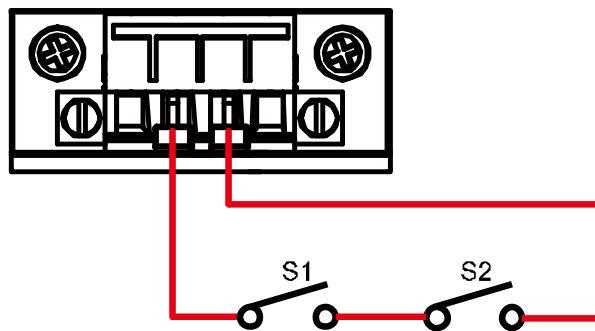

S1: Cage door switch by customer


S2: External switch by customer

Note: When both A and B are closed, the cabinet is powered on; if either A or B is disconnected, an emergency stop is triggered and the cabinet is powered off. If you need to power on the cabinet again, make sure that the switches at A and B are closed.

3. AC input power cable terminals for L1, L2, L3, and PE. (Hole size M8)

1.6 Home-Screen Overview



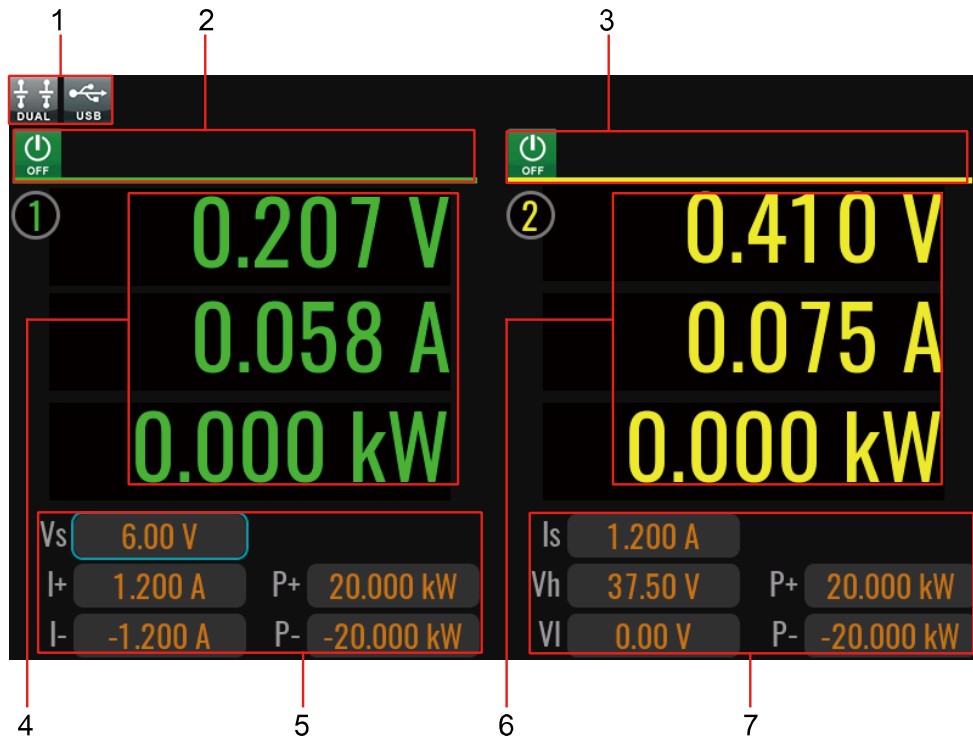






































IT6600 series power supply adopts touch screen design, the users can easily operation by touch screen. The details of the home screen are described below.



| No. | Name | Description |
|-----|----------------------------------|--|
| 1 | Power status bar | Displays the present output status. |
| 2 | CH1 status bar | Displays the output status of power channel 1. |
| 3 | CH2 status bar | Displays the output status of power channel 2. |
| 4 | Output values view area for CH1 | Displays the present output voltage, current and power values. |
| 5 | Setting values view area for CH1 | <ul style="list-style-type: none"> When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed. |
| 6 | Output values view area for CH2 | Displays the present output voltage, current and power values. |
| 7 | Setting values view area for CH2 | <ul style="list-style-type: none"> When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed. |

Introduction to Interface Symbols



The interface of IT6600 power supply will display the following symbols. All the symbols and description are listed in the table below.

| Char | Function description | Char | Function description |
|---|--|--|--|
| Shift | Compound key. |  | Output is off. |
|  | Output is on. |  | Key operation is locked. |
|  | The power supply is in a state of constant current output. |  | The power supply is in a state of constant voltage output. |
|  | The power supply is in a state of constant power output. |  | The power supply (Sink) is in constant resistance state. |
|  | The DV source is in remote mode. |  | Sense indicator. |
|  | 2-channel independent output mode. |  | Found USB disk. |
|  | 2-channel series mode. |  | 2-channel parallel mode. |
|  | LIST is running. |  | LIST is finished. |
|  | LIST function is waiting for trigger. |  | BAT is running. |
|  | BAT is finished. |  | BAT function is waiting for trigger. |
|  | BSIM is running. |  | BSIM is finished. |
|  | BSIM function is waiting for trigger. |  | DLOG is running. |
|  | DLOG is finished. |  | DLOG function is waiting for trigger. |
|  | ELOG is running. |  | ELOG is finished. |
|  | ELOG function is waiting for trigger. |  | Vehicle function is waiting for trigger. |
|  | Vehicle is running. |  | Vehicle is finished. |
|  | Standard is running. |  | Battery simulation mode. (under only load mode) |
|  | Only load mode. |  | Touch function is disabled. |
|  | SYNC lock |  | SYNC unlock |
|  | Fiber is error. |  | Output is disabled. |
|  | Over current protection. |  | Over temperature protection. |

| Char | Function description | Char | Function description |
|------|---|------|------------------------------|
| | Over voltage protection. | | Over power protection. |
| | Sense Error. | | Under current protection. |
| | Under voltage protection. | | Communication command error. |
| | Tip image is folded, click to expand all icons. | | Analogue Function |
| | Device calibration modes. | | Data recording function. |


Menu Introduction

Press the **[Menu]** key on the front panel and enter to the menu interface. Menu interface will display all of function icon, user can rotate the knob or direction key to select, or click the screen to enter the function interface.

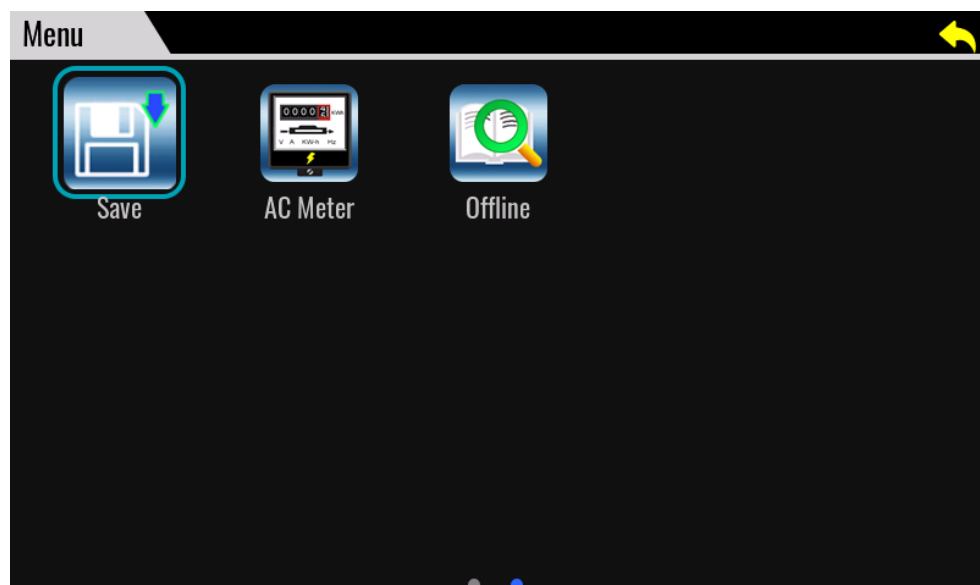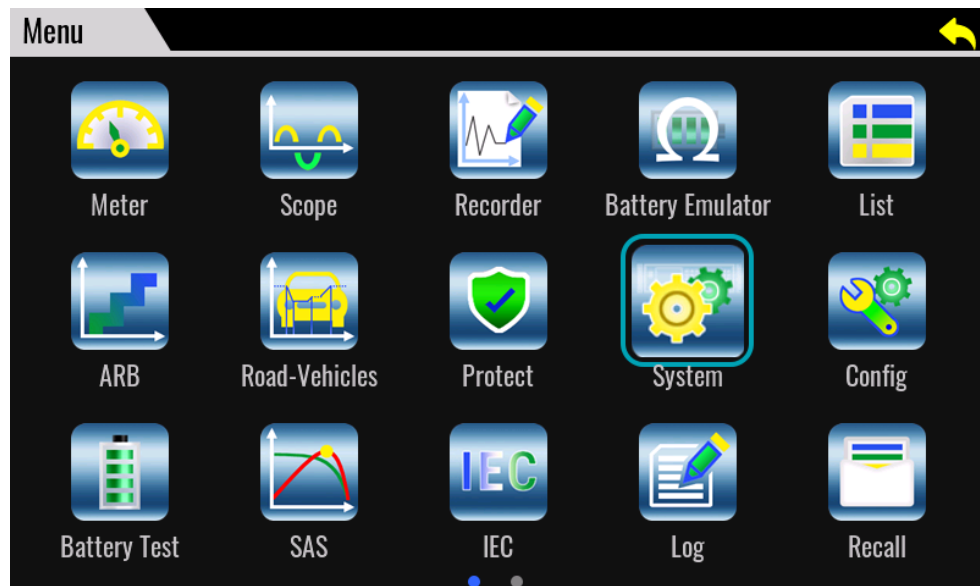

1.7 Instrument Installation and Dimensions

The instrument is equipped with air inlet and outlet vents at specific locations to ensure effective heat dissipation. When installing the instrument into a rack, make sure the airflow path remains unobstructed, and leave sufficient ventilation space around the cooling vents. Proper airflow direction must be maintained to ensure stable and reliable operation of the instrument. The following section provides an example using the 3U model.



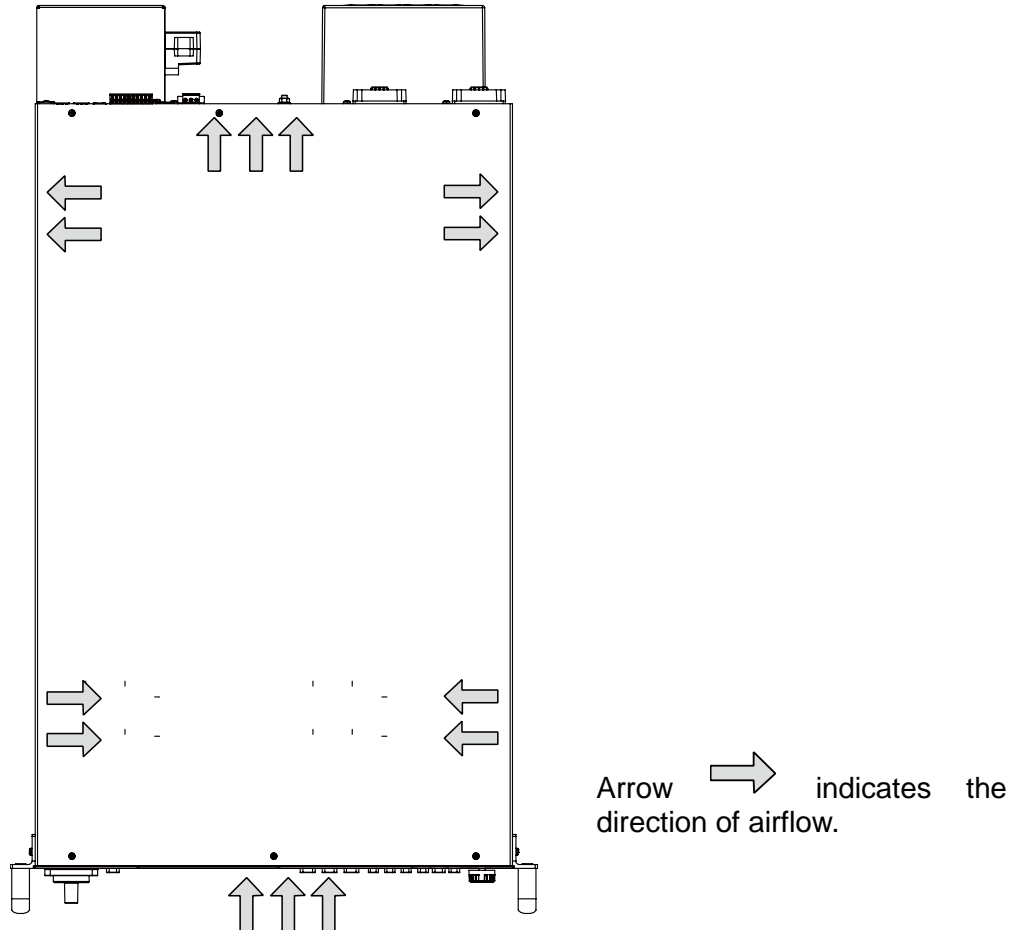


Installation Clearance Requirements for Standalone Units/Cabinets:



- **Rear Clearance:** The rear of the instrument must remain unobstructed. To ensure proper airflow and allow for the opening and closing of the rear door, the minimum clearance between the rear panel and the wall should be 1 meter.
- **Front Clearance:** The front of the instrument must remain unobstructed to allow for personnel access and adequate airflow for cooling. The minimum clearance between the front panel and the nearest wall or large surface should be 850 millimeters.
- **Side Clearance:** Both sides of the instrument should be free of obstructions. To ensure proper airflow, the minimum clearance between the side panels and the nearest wall or large surface should be 850 millimeters.

The detailed dimension drawings of the IT6600 series are as follows (unit:mm).


3U Model

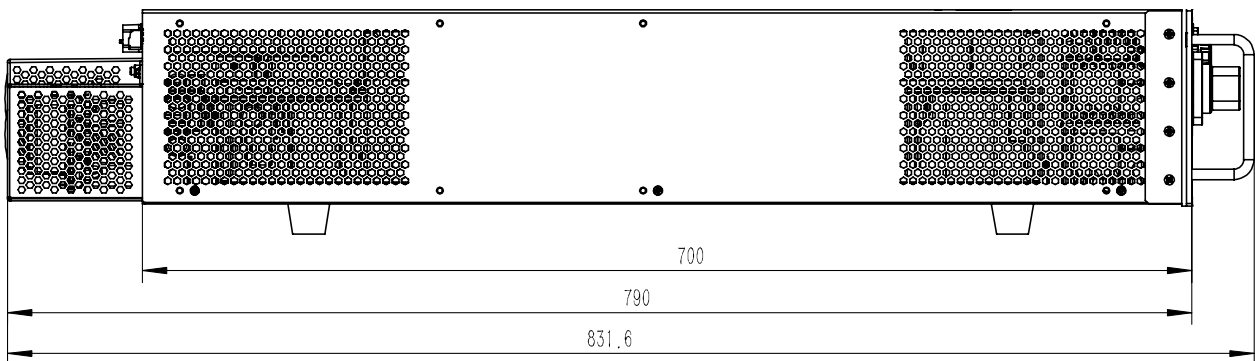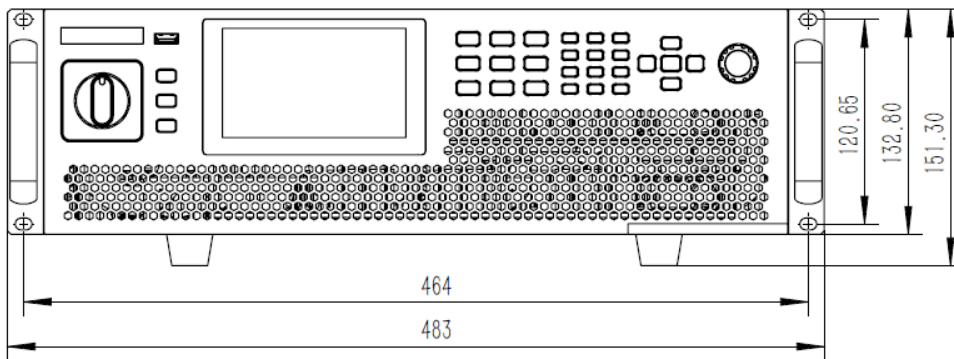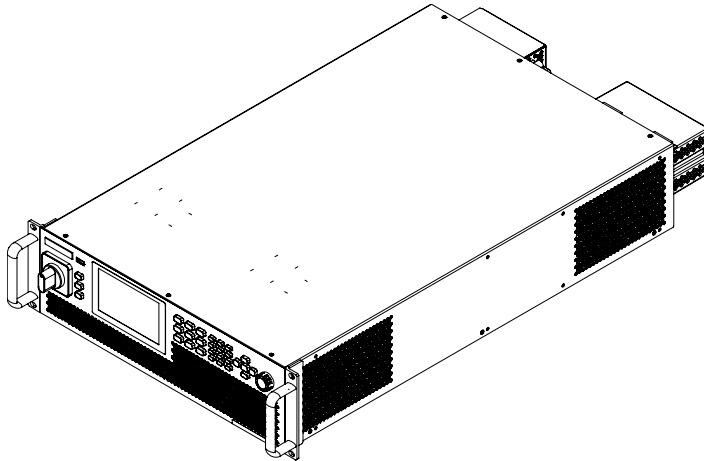


15U Model (One master and multi-slaves series)

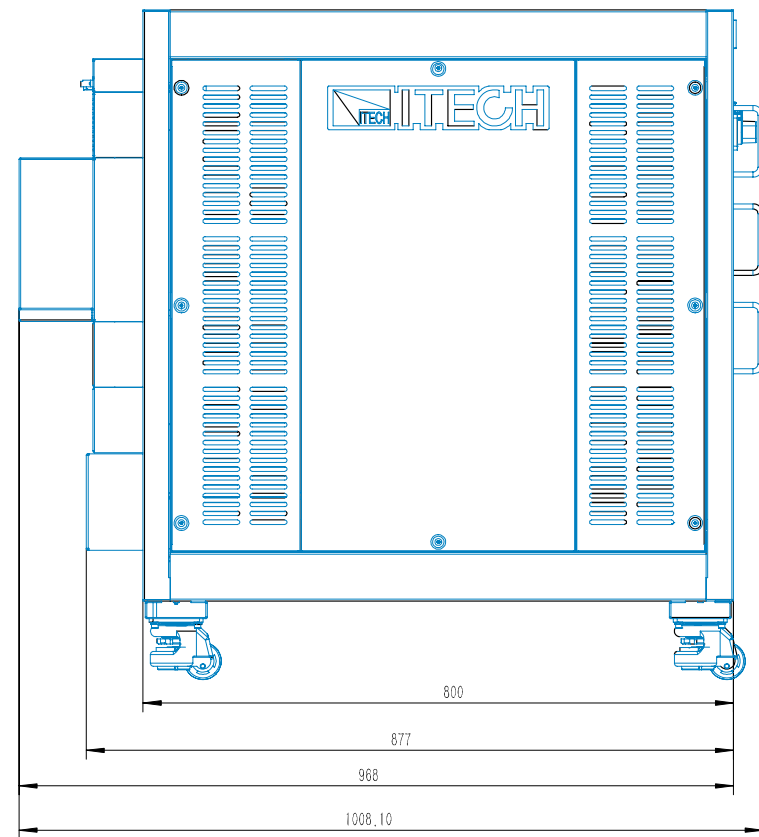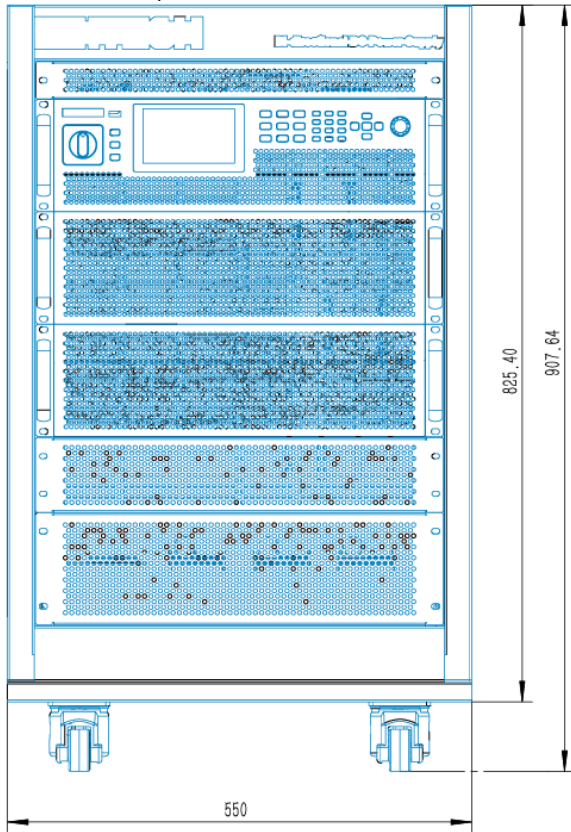



27U Model (One master and multi-slaves series)

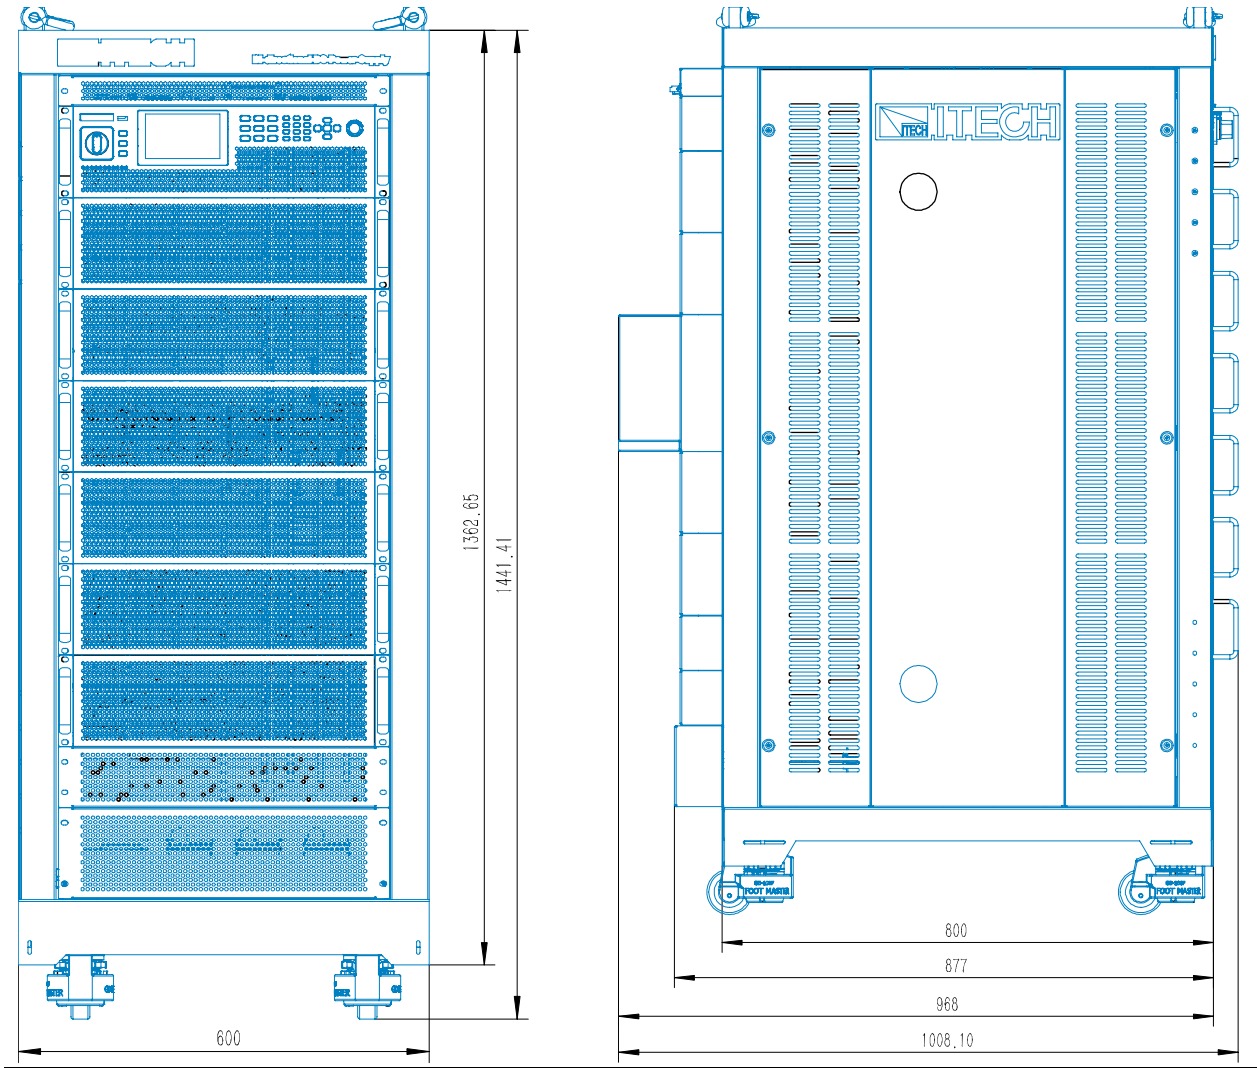


37U Model (One master and multi-slaves series)

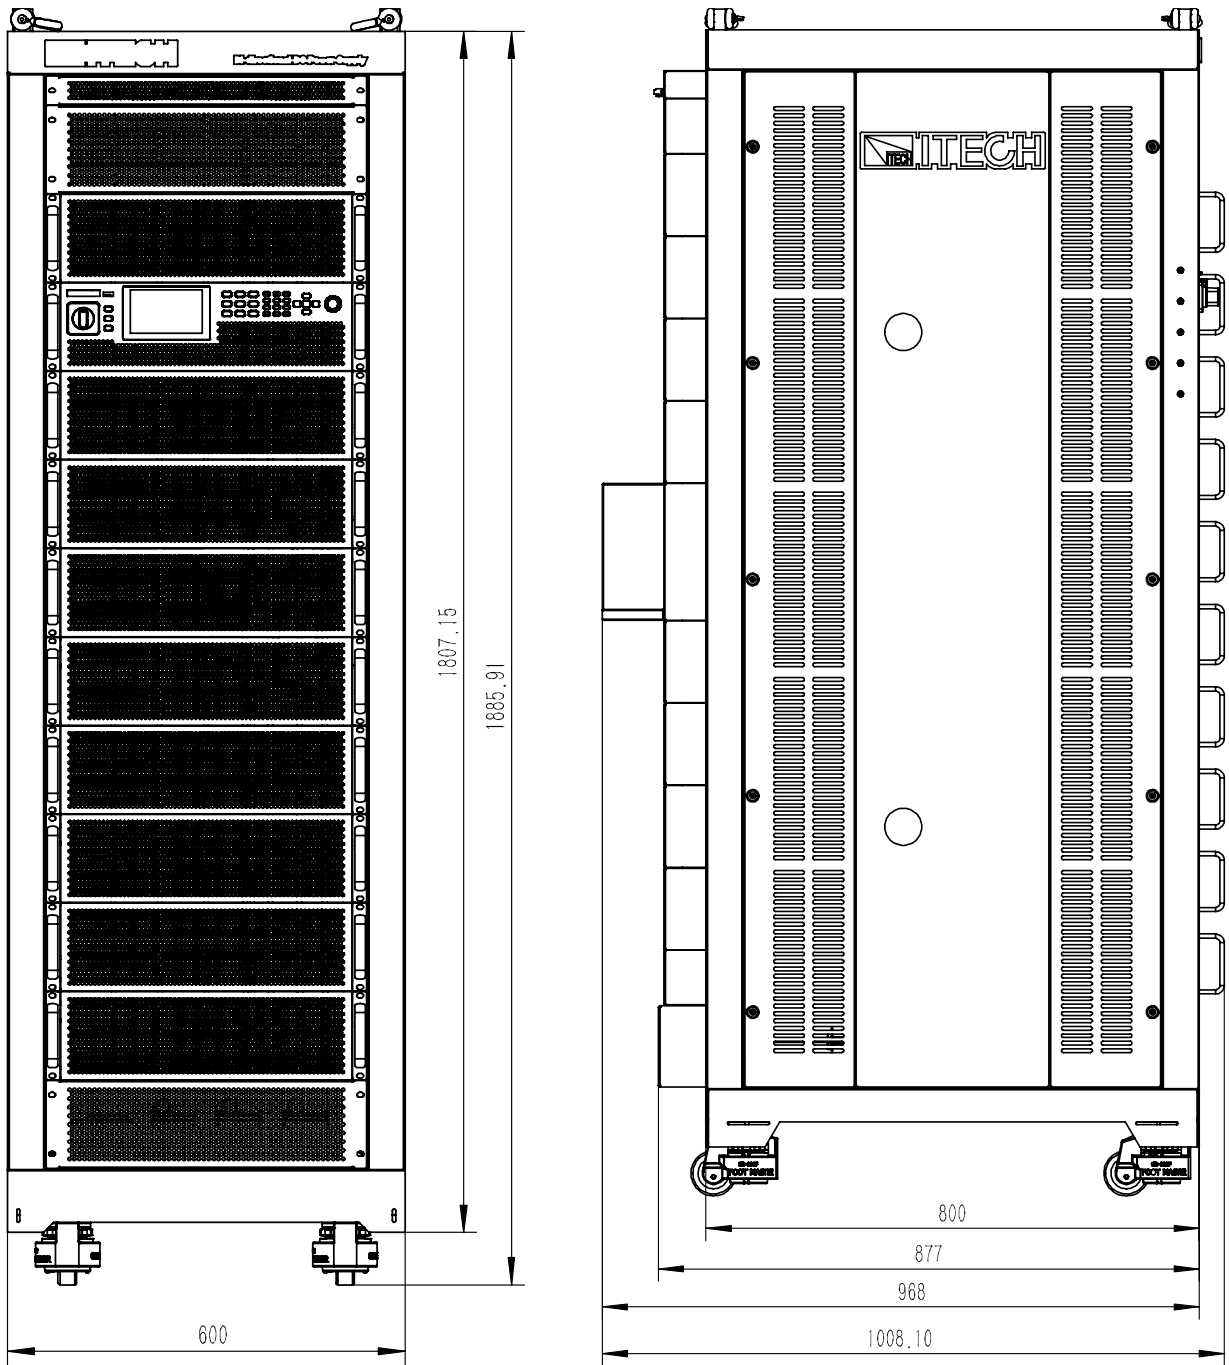


15U Model (Multi-masters series)

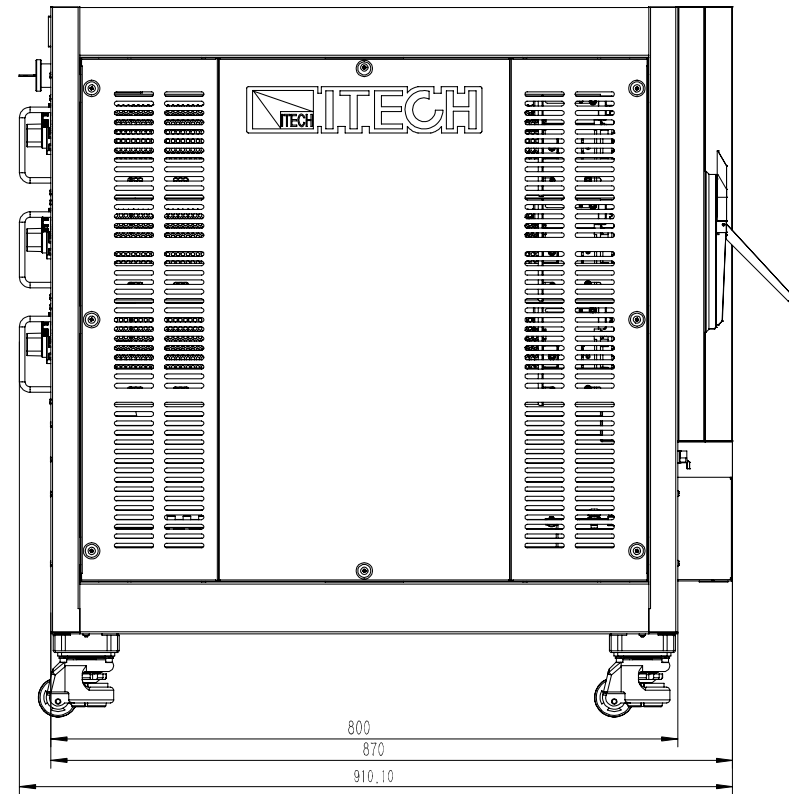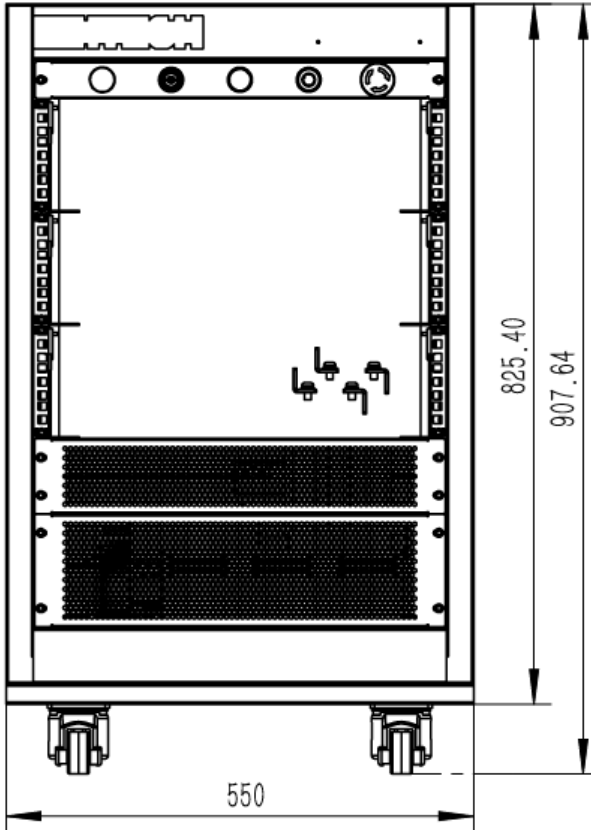

27U Model (Multi-masters series)

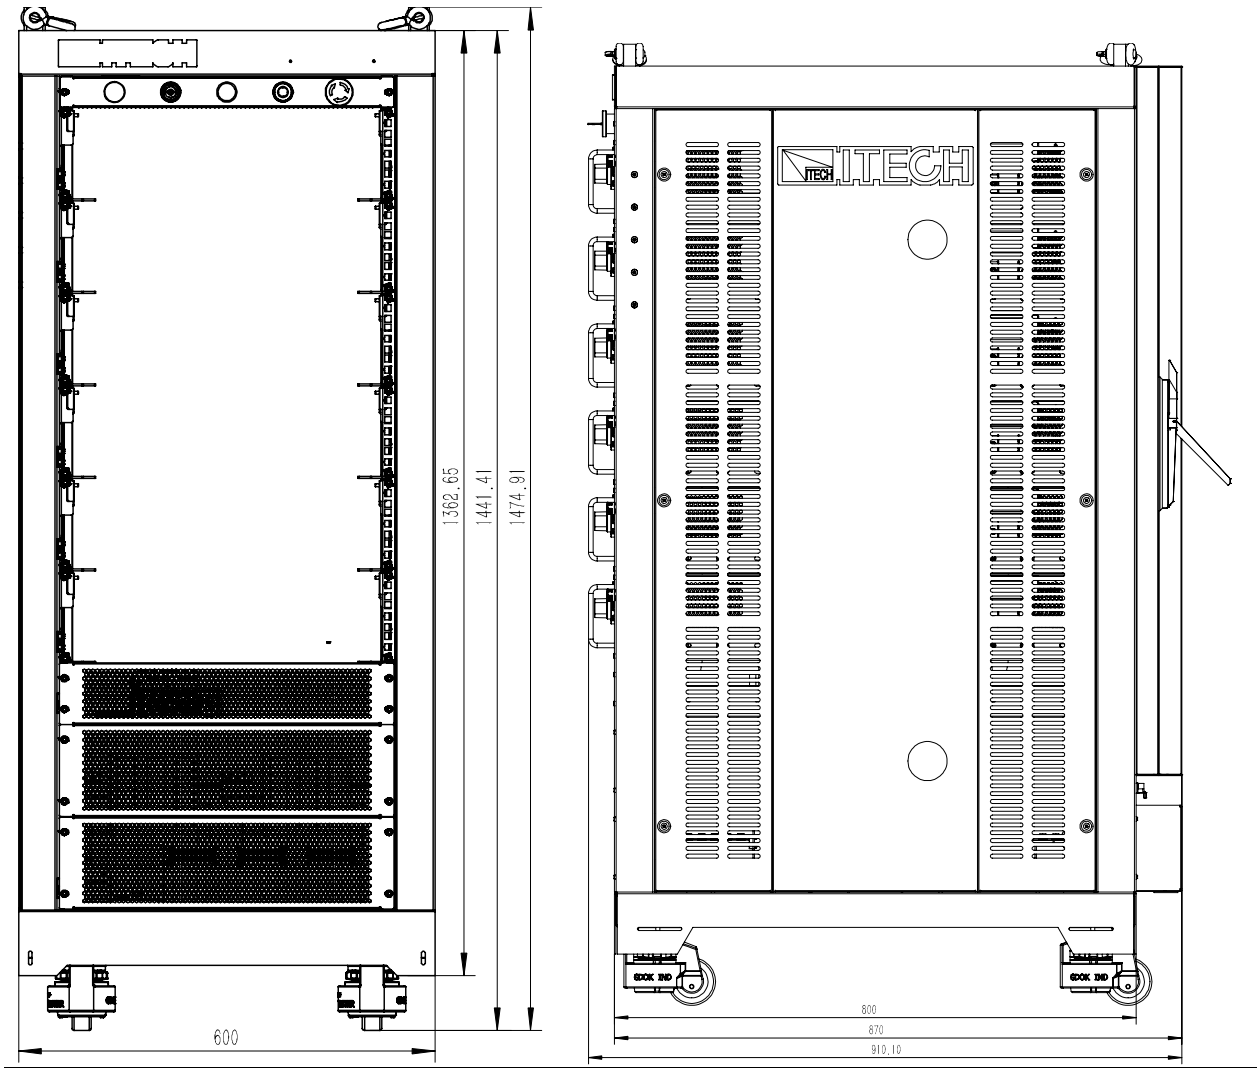

37U Model (Multi-masters series)

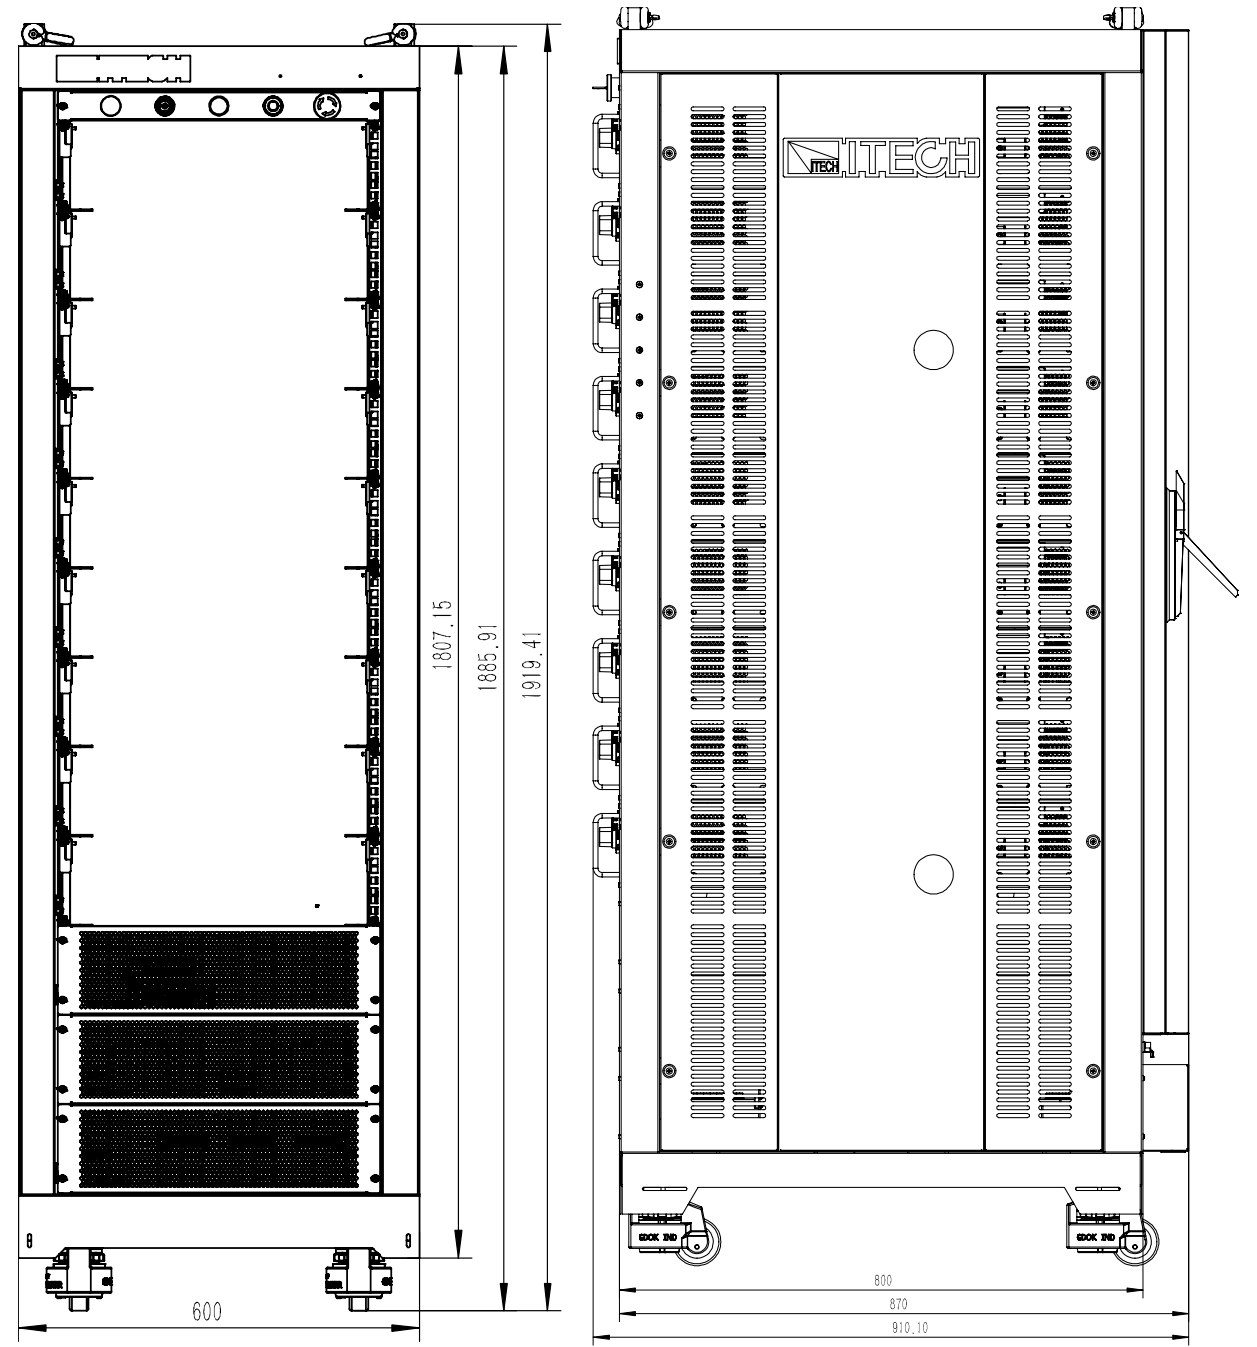

Chapter2 Inspection and Installation

2.1 Unpacking and Transportation

Unpacking





For cabinet products, they are packaged in wooden boxes at the factory. After you receive them, please refer to the unpacking instructions provided with the box for disassembly; for products packaged in cartons, please use appropriate tools for unpacking.

It is recommended to keep the complete transport packaging for the lifetime of the device for relocation or return to the manufacture for repair.

Cabinet Safety Symbols

A sticker bearing the following safety symbols is affixed to the upper left corner of the rear panel of the cabinet, as described below.



| Symbols | Introduction |
|---|--|
|  | General Warning <ul style="list-style-type: none"> ● Meaning: General warning, alerting personnel to potential hazards or important notices. ● Description: Indicates that the operation manual or safety instructions should be read to ensure awareness of potential risks. |
|  | Electric Shock Hazard <ul style="list-style-type: none"> ● Meaning: Risk of electric shock. ● Description: Indicates that high voltage or residual voltage may be present inside the equipment or at its terminals, posing an electric shock hazard if touched. |
|  | High Temperature Warning <ul style="list-style-type: none"> ● Meaning: High temperature warning. ● Description: The surface may become hot during operation and can cause burns if touched; protection should be used or contact should be avoided until cooled. |
|  | Tip-Over Hazard <ul style="list-style-type: none"> ● Meaning: Prevent equipment from tipping over or avoid collision-related injuries. ● Description: Indicates that the equipment may tip over during transport, relocation, or unstable installation, and anti-tip measures should be taken to prevent personal injury or equipment damage. |

Transportation

If you need to transport non-cabinet products, you must pay attention to the following to ensure the safety of equipment and personnel.


CAUTION

- Before moving, make sure that the cabinet or stand where the equipment will be placed has been fixed and meets the load-bearing conditions to avoid tilting and collapsing, causing personnel to be injured, and equipment broken.
- Due to the weight of the product, transport by hand should be avoided where possible. If unavoidable, carry it with two people and holding the product shell and not external parts (such as handles, electrodes, knobs, etc.).
- When carrying, be prepared to bear the weight to avoid sprains or being crushed by heavy objects.
- Use suitable safety clothing, especially safety shoes, when carrying the equipment, as due to its weight a fall can have serious consequences.

After unpacking the cabinet product, if you need to move it to other places, you must pay attention to the following matters to ensure the safety of equipment and personnel.

CAUTION

- The cabinet product is very heavy. Before moving to another location, confirm whether the ground load is in compliance.
- During the process of moving the cabinet, it is recommended that two or more people cooperate and push it slowly and at a constant speed. If you encounter a pit, you need to pay special attention. It is forbidden to push it quickly, otherwise it will easily cause excessive inertia and cause the casters at the bottom of the cabinet to jam and the cabinet to fall.
- It is not advisable to push down the slope to prevent the cabinet from falling down due to the shift of the center of gravity. It is recommended to use a forklift or crane to move the cabinet.
- ITECH 27U and 37U cabinets are equipped with hoisting rings as standard on the top. It is recommended to use a crane equipped with a four-leg hoisting belt structure for horizontal hoisting and moving, and ensure that the four hoisting belts are the same length to avoid cabinet skew during movement. As shown below.
- After moving to the destination, please lock the four casters to secure the cabinet.
- The cabinet should be placed on a level ground. It is forbidden to place the cabinet on a sloped ground.

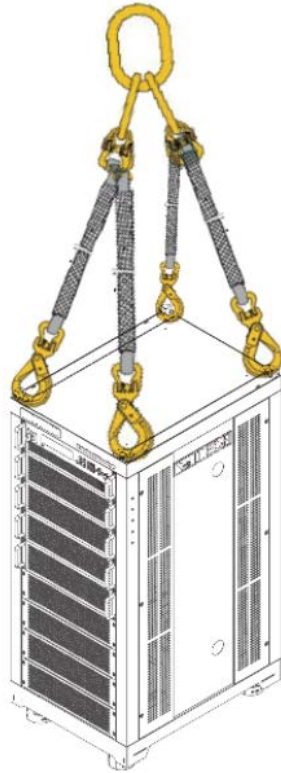

2.2 Verifying the Shipment

Open the package and check the articles within package box before operation. In case of any non-conformity, missing or appearance wearing, please contact ITECH immediately.

The package box should comprise:

| Device name | Quantity | Model | Remarks |
|--|----------|---------------|--|
| High-power DC Power Supply | x1 | IT6600 series | For the specific models included in this series, refer to 1.2 Models and Options . |
| Power Cord | - | - | The 3U models come standard with one power cord; the 15U models come with one set of power cords; the 27U and 37U models each come with two sets of power cords. |
| USB communication cable | x1 | - | This is used when the USB interface is used for starting up remote operation. |
| LAN communication cable | x1 | - | This is used when the LAN interface is used for starting up remote operation. |
| Busbar Kits for Parallel-Series connection | x1 | IT-E184 | Used for connecting machines in series or parallel. (Standard on 3U models only.) |
| Calibration Report | x1 | - | It is the calibration certificate of the instrument before delivery. |


NOTE

After confirming that package contents are consistent and correct, please appropriately keep package box and related contents. The package requirements should be met when the instrument is returned to factory for repair.

2.3 Connecting the Power Cord

Connect power cord of standard accessories and ensure that the power supply is under normal power supply.

Before connecting the power cord

To prevent electric shock and damage to the instrument, observe the following precautions.

WARNING


- Before connecting power cord, be sure to confirm that the power voltage matches with the rated input voltage of the instrument.
- Before connecting power cord, be sure to switch off the instrument. Verify that there is no dangerous voltage on the connection terminals.
- To avoid fire or electric shock, Make sure to use the power cord supplied by ITECH.
- Be sure to connect the power cord to the AC distribution box with protective grounding. Do not use terminal board without protective grounding.
- Do not use an extended power cord without protective grounding, otherwise the protection function will fail.
- Ensure that the power cord connection terminals are either insulated or covered by the supplied protective cover so that no accidental contact with lethal voltage can occur.

CAUTION

Safety agency requirements dictate that there must be a way to physically disconnect the AC mains cable from the unit. A disconnect device, either a switch or circuit breaker must be provided in the final installation. The disconnect device must be close to the equipment, be easily accessible, and be marked as the disconnect device for this equipment.

Categories of Power Cords

- 3U instruments provides the standard power cords as below.

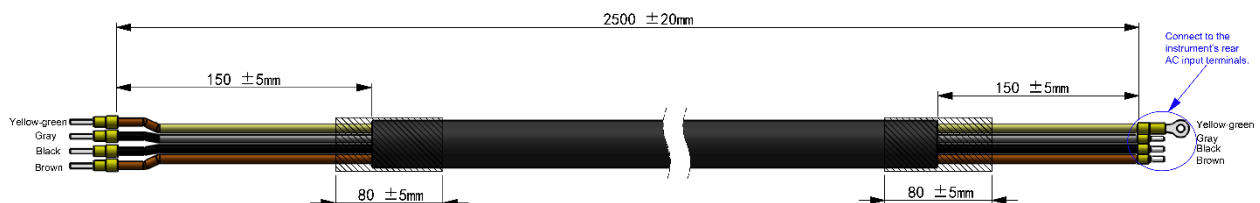


The yellow-green wire is grounding wire, which is connected to the PE terminal of power input on the rear panel; the others are live wires, which are correspondingly connected to the L1, L2 and L3 terminals of power input on the rear panel of the instrument.

The power cord specification for the 3U instruments is $4 \times \text{AWG } 3 / 105^\circ\text{C}$ /

2500 mm.

- This series of 15U cabinets comes standard with one set, and the 27U and 37U cabinets come standard with two sets of 2.5-meter AC input power cords (each set contains four cords). Each cord is shown below.

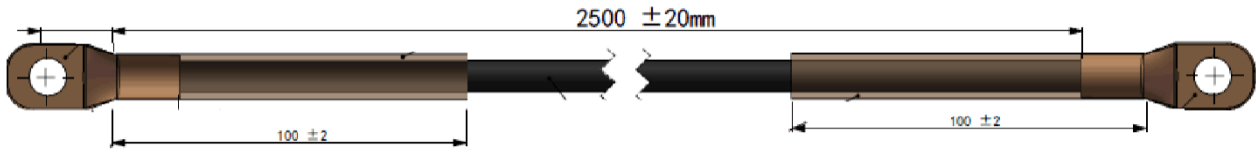

The yellow-green wire is grounding wire, which is connected to the PE terminal of power input on the rear panel; the others are live wires, which are correspondingly connected to the L1, L2 and L3 terminals of power input on the rear panel of the instrument.

The specifications of the power cords are shown in the table below.

| Cabinet Height | Number of Power Cords (sets) | Cords Specification |
|----------------|------------------------------|--|
| 15U | 1 set | AWG 2 / 600V / 105°C, crimped with TLK35-10 terminals on both ends. |
| 27U | 2 sets | AWG 3/0 / 600V / 105°C, crimped with TLK95-10 terminals on both ends. |
| 37U | 2 sets | AWG 4/0 / 600V / 105°C, crimped with TLK120-10 terminals on both ends. |



NOTE


The colors of the L1/L2/L3 cables vary by region; for example, in Europe, they are brown, black, and grey.

AC Power Input Level

The AC input of this series is a three-phase AC power (three-phase four-wire) by default, the detailed specifications refer to Technical Specifications.


Connecting the Power Cord

The AC input is three phase and balanced, connecting the power cord as below.

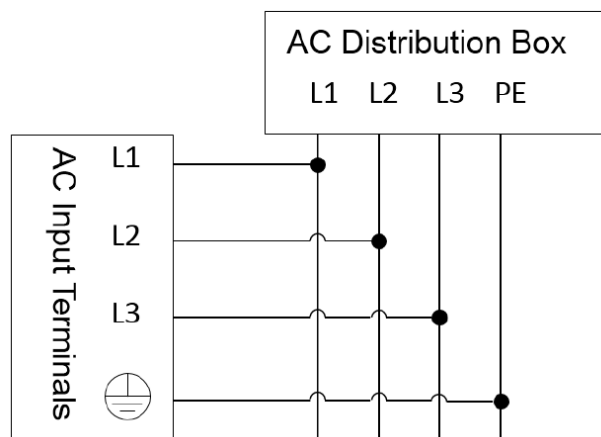

Operation procedures:

1. Confirm that the switch of the AC power distribution box is off.
2. Confirm that the power switch is in the OFF position and verify that there is no dangerous voltage on the connection terminals.
3. Connect the end of the power cord with the round terminal (ground terminal) to the AC power input terminal on the rear panel of the instrument.
 - a) You only need to connect the brown/black/gray live wires to the terminals on the rear panel, which are not required to correspond to L1, L2 and L3 terminals one by one.
 - b) The yellow-green wire is grounding wire, which is connected to the protective grounding terminal (PE).

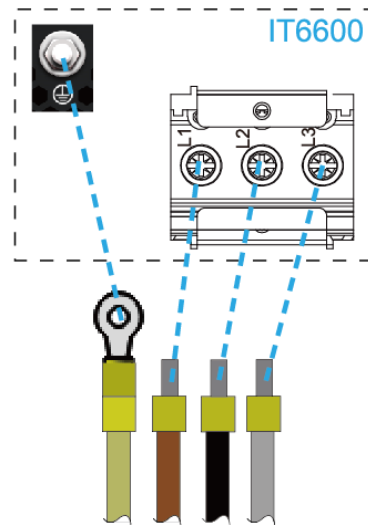

4. Refer to the suggestion connection diagram, connect the other end of the power cord to the required AC distribution box.

Connect the 2 sets of power cords for the 27U/37U models to the AC distribution box.

2.4 Connecting Test Lines (Optional)

Test lines are not standard accessories of the instrument. Please select optional red and black test lines for individual sales based on the maximum current value. For specifications of test lines and maximum current values, refer to “**Specifications of Red and Black Test Lines**” in “**Appendix**”.

WARNING

- Before connecting test cables, be sure to switch off the instrument. Power switch is in Off position, otherwise touching the output terminals on the rear panel may result in personal injury or death due to electric shock.
- To avoid electrical shock, before testing, please make sure the rating values of the testing cables, and do not measure the current that higher than the rating value. All test cables shall be capable of withstanding the maximum short circuit current of the instrument without causing overheat.

- If several loads are provided, each pair of load wires shall safely withstand the rated short circuit output current of the power supply under full load.
 - Do not short the battery when connecting or disconnecting the battery testing circuit. Short circuit may cause severe accident.
 - Because the instrument can be used to sink current, hazardous voltages from an external energy source such as a battery may be present on the output terminals even with the instrument power off. Provision must be made to disconnect the external energy source before touching the output or sense terminals.
 - Always use test cables provided by ITECH to connect the equipment. If test cables from other factories are used, please confirm the maximum current that the test cables can withstand.
 - During wiring, check that the positive and negative poles of the test cables are properly and tightly connected. Do not connect the positive pole and disconnect the negative pole.
 - It is recommended that for battery testing, a fuse must be connected in series between the power supply and the battery to prevent short circuits caused by any problems.
 - When connecting the DUT (including but not limited to battery/capacitor), it is recommended that you purchase the IT-E165A anti-reverse connection module to prevent the battery/capacitor reverse connection that may cause damage to the instrument; When there is no external auxiliary equipment connected to prevent reverse connection and anti-spark function, please pay attention to the safety of the wiring, and be careful not to reverse the battery/capacitor connection, reverse connection will cause damage to the instrument, even if it is not powered on.
 - Ensure that the output terminals are either insulated or covered using the safety covers provided, so that no accidental contact with lethal voltages can occur.
 - For energy conservation, make sure to shut down the instrument and any temperature control equipment (e.g., air conditioners) after use.
-

Specification for Test Cables

Test cables are not standard accessories for the instrument. Please select optional red and black test cables for individual sales based on the maximum current value. For specifications of test cables and maximum current values, refer to [Specifications of Red and Black Test Cables](#) for more information.

Electrode introduction

The wiring apertures on the DC electrodes of the 3U model and the cabinet model are both **M8**.


Connecting the DUT (Local Measurement)

The instrument supports two kinds of wiring methods with the DUT: local

measurement and remote measurement (SENSE). The default test mode is local measurement.

Please confirm that the Remote Sense function in the menu is set to Off, otherwise the instrument will report an error in the present connection mode.

The connection diagram and steps of local sensing are as follows.

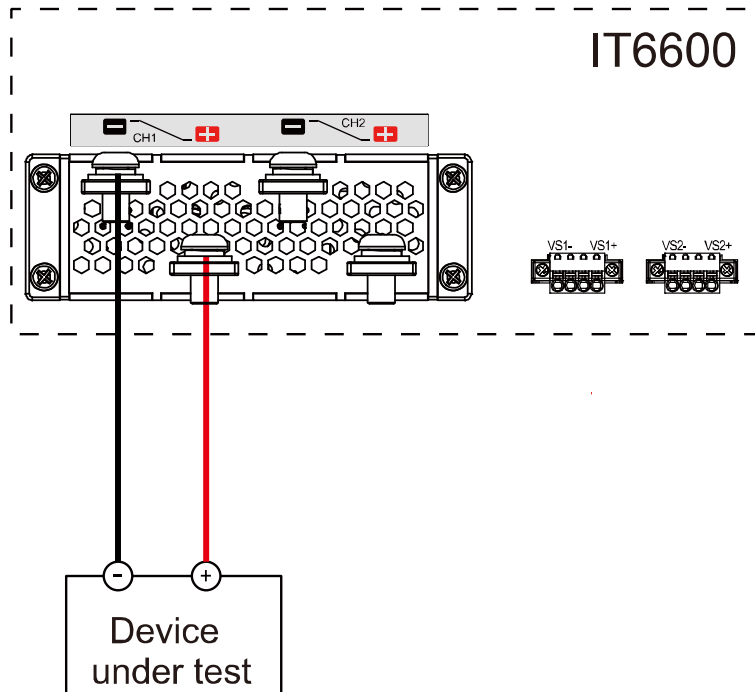

1. Confirm that the power switch is in the OFF position and verify that there is no dangerous voltage on the connection terminals.
2. Remove the output terminals cover of the power system.
3. Loosen the screws of the output terminals and connect the red and black test cables to the output terminals. Re-tighten the screws.

When maximum current that one test cable can withstand fails to meet the rated current, use multiple pieces of red and black test cables. For example, the maximum current is 1,200A, then 4 pieces of 360A red and black cables are required.

4. Thread the red and black test cables through the output terminals cover of the power system and install the cover.
5. (Optional) According to the actual situation of DUT, connect the grounding terminal on the rear panel of the instrument to the DUT to ensure the safe grounding.

For the location information, see 1.5 Rear Panel.

6. Connect the other end of the red and black cables to the DUT. The positive and negative poles must be properly connected and fastened when wiring.

Connecting the DUT (Remote Sensing)

Remote measurement is available for the following scenarios:


When the DUT consumes large current or the wires are too long, there is a voltage drop on the wires between DUT and output terminals of the power system.

To maximize measurement accuracy, the power system provides the remote measurement terminals VS+ and VS- on the rear panel, which can be used to

measure the terminal voltage of the DUT.

When the power system is used for battery testing in actual applications, the voltage drop of the wire will lead to voltage inconsistency of both ends and inconsistency of the cutoff voltage of power system and the actual voltage of battery, resulting in inaccurate measurement.

The connection diagram and steps of remote measurement are as follows:

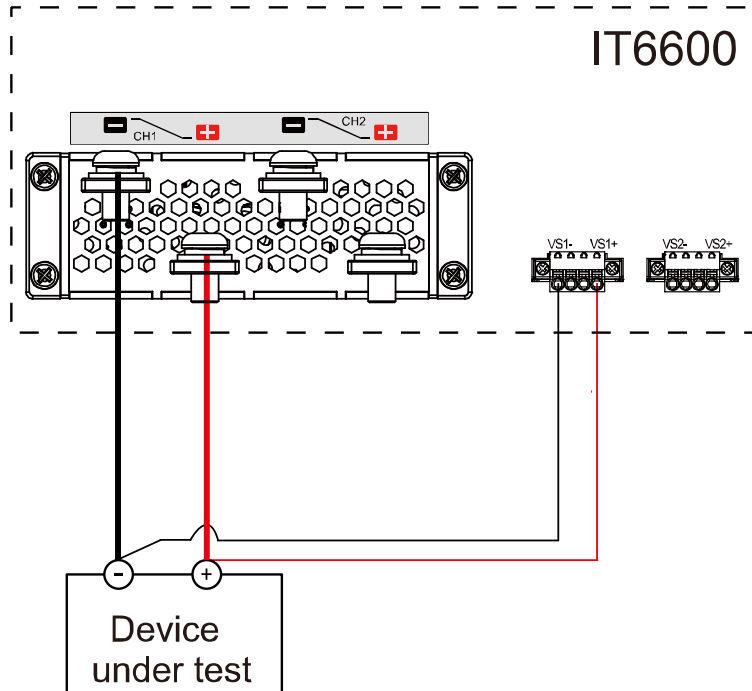

1. Confirm that the power switch is in the OFF position and verify that there is no dangerous voltage on the connection terminals.
2. Remove the output terminals cover of the power system.
3. Refer to the wiring diagram and connect the Vs+ and Vs- with armored twisted-pair cables. Loosen the screws of the output terminals and connect the red and black test cables to the output terminals. Re-tighten the screws.

When maximum current that one test cable can withstand fails to meet the rated current, use multiple pieces of red and black test cables. For example, the maximum current is 1,200A, then 4 pieces of 360A red and black cables are required.

4. Thread the red and black test cables through the output terminals cover of the power system and install the cover.
5. (Optional) According to the actual situation of DUT, connect the grounding terminal on the rear panel of the instrument to the DUT to ensure the safe grounding.

For the location information, see [1.5 Rear Panel](#).

6. Connect the other end of the remote sense cables to the DUT.
7. Connect the other end of the red and black cables to the DUT. The positive and negative poles must be properly connected and fastened when wiring.
8. Power on the instrument and turn on the **Remote Sense** function of the instrument.

Chapter3 Getting Started

3.1 Power-on the Instrument

A successful selftest indicates that the purchased power product meets delivery standards and is available for normal usage.

Before operation, please confirm that you have fully understood the safety instructions.

Precautions

To prevent electric shock and damage to the instrument, please observe the following precautions.

WARNING

- Before connecting power cord, be sure to confirm that the power voltage matches with the supply voltage.
- Before connecting power cord, be sure to switch off the instrument. Verify that there is no dangerous voltage on the terminals before touching them.
- To avoid fire or electric shock, make sure to use the power cord supplied by ITECH.
- Be sure to connect the main power socket to the power outlet with protective grounding. Do not use terminal board without protective grounding.
- Do not use an extended power cord without protective grounding, otherwise the protection function will fail.
- Ensure that the input electrodes are either insulated or covered using the safety covers provided, so that no accidental contact with lethal voltages can occur.
- If you notice strange sounds, unusual odors, fire, or smoke around or from inside the instrument, flip the POWER switch to the (O) side to turn the instrument off, or remove the power cord plug from the outlet. The detachable power cord may be used as an emergency disconnecting device. Removing the power cord will disconnect AC input power to the unit.

CAUTION

Safety agency requirements dictate that there must be a way to physically disconnect the AC mains cable from the unit. A disconnect device, either a switch or circuit breaker must be provided in the final installation. The disconnect device must be close to the equipment, be easily accessible, and be marked as the disconnect device for this equipment.

Power Switch Introduction

User can adjust the switching knob directly to turn on or turn off the device. The status of switching knob is as follows.

When the switching knob is in the OFF position, it can be rotated 90 degrees clockwise to power on the device; when the switching knob is in the ON position, it can be rotated 90 degrees counterclockwise to power off the device.



Turning the POWER Switch On

Check that the power cord is connected properly.

Flip the POWER switch to the (ON) side to turn the instrument on. The front panel display will light up after a few seconds. It may take about 30 seconds or so for the power supply to initialize before it is ready for use.

If a self-test error occurs, an error message will be displayed in the front panel. Press the **[Esc]** button to try to clear the current fault status. The user can also restart the instrument to try to clear the fault status. Wait until the power is turned off and then start again. If the problem still cannot be solved after restarting, please contact the ITECH engineer.

Turning the POWER Switch Off

Flip the POWER switch to the (OFF) side to turn the instrument off. When it is turned off, the instrument interface will prompt "Please wait for the device power down.", and the instrument will store the setting information before shutdown in the group 1 nonvolatile memory.

After you turn the POWER switch off, wait at least 10 seconds after the fan stops before you turn the POWER switch back on. Turning the instrument on too soon after you turn it off can cause damage to the inrush current limiter circuit, as well as reduce the life of components such as the POWER switch and the internal input fuses.

3.2 Touch Screen Introduction

This series of power display is a touch screen LCD interface, users can select and set parameters by hand touch. The touch function can be set in the system menu.

This parameter determines the state of the touch screen.

1. Press the **General** under the system menu.
2. Press the Up/Down key or turn the knob to select the **Touch Function** and press **[Enter]**.
 - On: enable touch function.
 - Off: disable touch function.

3.3 Set output parameters

The voltage value and current value can be programmed, which can be set to different parameters within the specification range based on customer requirements. This can meet various test requirements of the customer.

After the user presses the **[V-set]** or **[I-set]** keys on the front panel, the instrument interface displays the parameters to be set and the cursor flashes for prompt. The user can use the following methods to set the values.

- Directly use the number keys to set the value.
- Rotate the knob to set the data in the cursor position. Rotate the knob lockwise to increase the set value and anticlockwise to decrease the set value. Once the data in the cursor position increases to ten, the value will add one to the front position automatically. and once the data in the cursor position decreases to zero, the value will minus one from the front position automatically. This provides convenience for the user to set. The knob can works with the left or right keys. Use the left or right keys to move the cursor position.

 **NOTE**

After entering the menu interface, the knob can also be used to scroll pages to view menu items.

3.4 Output On/Off Control

WARNING

- The **[On/Off]** key is used to turn the output on or off under normal circumstances. Even if the instrument is in control by PC or the keyboard is locked, the **[On/Off]** is still valid.
- The **[On/Off]** key light is off and turning the output off does not place the instrument in a safe state. Hazardous voltages may be present on all output and guard terminals. Putting the equipment into an output-off state does not guarantee that the outputs are powered off if a hardware or software fault occurs. See the cautions about connecting the test lines before connecting test lines.

Controlled by the **[On/Off]** key

User can control the output switching of the instrument's 2 channels by pressing the **[CH1 On/Off]** key and the **[CH2 On/Off]** key on the front panel. If the **[On/Off]** key light is on, indicates that the output is turned on. The meter area on the interface will display the voltage, current, and power values in the current circuit. If the **[On/Off]** key light is off, indicates that the output is turned off. The LCD displays that the power supply state is OFF.

Controlled by Digital IO pins

The Digital IO pin, which comes standard with this series of instruments, supports external level/pulse signal control output, and in combination with external circuitry, enables emergency stop control of the output. Refer to the following use case.

Case:

Pin 5 of Digital IO has an INTERLOCK function. In the default settings of **Reverse (Off)** and **Inhibit-Living**, pulling pin 5 low (0V) can disable the machine's output. At this point, the **[On/Off]** key light is on, but there will be no

actual output. Restoring pin 5 to a high level will resume normal output from the machine.

1. Go to the **System**→**IO**→**Digital IO-5 Settings** menu.
2. Select the **Reverse(Off)** and **Inhibit-Living** items, and press [Enter] to confirm.
3. Connect Pin5 (positive) and Pin8 (negative) of Digital IO to the external signal control circuit.

At this time, 5V is output between Pin5 and Pin8.

4. After connecting the DUT, turn on **[On/Off]**.
5. Input 0V to Pin5 (positive) and Pin8 (negative), or directly short Pin5 and Pin8.

At this point, output is disabled.

6. Input 5V to Pin5 (positive) and Pin8 (negative), or disconnect the short wire between Pin5 and Pin8.

At this point, output is restored.

Chapter4 Power Supply Function

This chapter describes the functions and features of the power supply.

4.1 Source Mode/ Load Mode Switch

The IT6600 series integrates bidirectional power supply and regenerative load functional characteristics in one unit for continuous supply and absorption of current. It not only can realize the function of power source, but also capable of sink to load current, that realize the fast and continuous seamless switching between output and sink current , to effectively avoid voltage or current overshoot.

The switching mechanism between source mode and load mode is determined solely by the set voltage value of the power supply and the actual value at the power output terminal.

- **Source Mode:** When the set voltage value of the IT6600 is higher than the actual voltage of the externally connected product under test, the IT6600 will operate in Source mode.
- **Load Mode:** When the set voltage value of the IT6600 is lower than the actual voltage of the externally connected product under test, the IT6600 will operate in load mode.

4.1.1 Source Mode

This series of instruments supports Constant Voltage (CV), Constant Current (CC), and Constant Power (CP) output modes under Source Mode. The power supply operates in the mode that produces the minimum calculated output current.

In CV mode, the output current is determined by $I=U/R$, and in CP mode, it is determined by $I=\sqrt{(P/R)}$, where R is the equivalent load impedance of the DUT (Device Under Test).

When CV mode has priority:

Instrument settings: Voltage setting value (V_s), current upper limit value (I_+), power upper limit value (P_+).

- If $(V_s/R) > I_+$ and $\sqrt{(P_+)/R} > I_+$, the instrument operates in **CC mode**.
- If $I_+ > (V_s/R)$ and $\sqrt{(P_+)/R} > (V_s/R)$, the instrument operates in **CV mode**.
- If $(V_s/R) > \sqrt{(P_+)/R}$ and $I_+ > \sqrt{(P_+)/R}$, the instrument operates in **CP mode**.

When CC mode has priority:

Instrument settings: Current setting value (I_s), voltage upper limit value (V_h), power upper limit value (P_+).

- If $(V_h/R) > I_s$ and $\sqrt{(P_+)/R} > I_s$, the instrument operates in **CC mode**.
- If $I_s > (V_h/R)$ and $\sqrt{(P_+)/R} > (V_h/R)$, the instrument operates in **CV mode**.
- If $(V_h/R) > \sqrt{(P_+)/R}$ and $I_s > \sqrt{(P_+)/R}$, the instrument operates in **CP mode**.

4.1.2 Only load mode

This series supports setting the power supply to only load mode and can be tested with load in CR, CC, and CP modes. The usage of this function is as follows:

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.
2. Press the up/down key or rotate the knob to find **Priority Mode** menu.
 - i. Press the up/down key to move the cursor to the Mode function setting and press the **[Enter]** key to confirm. Rotate the knob to set **CC** priority, and press the **[Enter]** key to confirm.
 - ii. Press the up/down key to move the cursor to the **Only Load** function setting and press the **[Enter]** key to confirm. Rotate the knob to select On, and press the **[Enter]** key to confirm.
3. Press **[Esc]** to return to the main interface.

Users can set the constant current value (Is), constant resistance value (Rs), and constant power value (Ps) in load mode.

The power supply works in the mode that yields the minimum sink current value (calculated value). In constant resistance mode, the instrument's sink current is determined by $I=U/R_s$, while in constant power mode, the sink current is determined by $I=Ps/U$. Here, U represents the output voltage of the Device Under Test (DUT).

4. Set the DUT (power supply) to output 100V, 50A.
 - If $I_s = -10A$, $R_s = 5\Omega$ (sink current is $100/5 = 20A$), and $P_s = 3000W$ (sink current is $3000/100 = 30A$), the actual sink current is 10A. In this case, the instrument is working in CC mode.
 - If $I_s = -10A$, $R_s = 20\Omega$ (sink current is $100/20 = 5A$), and $P_s = 3000W$ (sink current is $3000/100 = 30A$), the actual sink current is 5A. In this case, the instrument is working in CR mode.
 - If $I_s = -10A$, $R_s = 5\Omega$ (sink current is $100/5 = 20A$), and $P_s = 800W$ (sink current is $800/100 = 8A$), the actual sink current is 8A. In this case, the instrument is working in CP mode.

4.1.3 Battery simulation mode

This series instrument **only load** mode comes with a battery simulation mode, which is applicable to discharge function test for the charger. The user can directly select this mode in the configuration menu.

In the charging principle of charger, after the charger is connected to the battery, monitor the battery voltage at first. If the battery connection is reliable and correct, the charger enters the charging state. When the instrument is under the battery simulation mode of load, an simulate battery voltage can be set, which has weak output capacity capable of outputting small current for simulating battery state. Thus, the charger's working requirements can be met.

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.
2. Press the up/down key or rotate the knob to find **Priority Mode** menu.
 - i. Press the up/down key to move the cursor to the Mode function setting and press the **[Enter]** key to confirm. Rotate the knob to set **CC** priority, and press the **[Enter]** key to confirm.
 - ii. Press the up/down key to move the cursor to the **Only Load** function setting and press the **[Enter]** key to confirm. Rotate the knob to select

On, and press the **[Enter]** key to confirm.

- iii. Press the up/down key to move the cursor to the **Battery Simulation** function setting and press the **[Enter]** key to confirm. Rotate the knob to select On, and press the **[Enter]** key to confirm.
3. Press **[Esc]** to return to the main interface.

The user can set the voltage value V_s , the resistance value R_s , the upper limit of input current I_s and the upper limit of input power P_s to simulate battery.

NOTE

When the instrument is under the battery simulation mode of load, the loaded current limit is the maximum current value of the model. The user does not need to set small current for external output, the size of which has been defined in the instrument.

4.2 Output Function

4.2.1 Set the Output Mode

The IT6600 series power supply supports DC output mode. The output mode can be select in the config menu.

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.
2. Press the up/down key or rotate the knob to find **Output Couple Mode** menu.
 - i. Press the up/down key to move the cursor to the Mode function setting and press the **[Enter]** key to confirm. Rotate the knob to set DC output mode, and press the **[Enter]** key to confirm.
3. Press **[Esc]** to exit.


DC Mode

When the DC is turned on, it indicates that the instrument serves as a DC power supply. Under this mode, the instrument will generate DC output. The default set of IT6600 series power supply is DC Mode.

Set the Output Voltage/Current/Power

- In CV priority (default) mode, the main interface displays V_s (Setting value of voltage), I_+ (Upper limit of current), I_- (Lower limit of current), P_+ (Upper limit of power), and P_- (Lower limit of power).
- In CC priority mode, the main interface displays I_s (Setting value of current), V_h (Upper limit of voltage), V_l (Lower limit of voltage), P_+ (Upper limit of power), and P_- (Lower limit of power).

Press the up/down key to move the cursor to the **parameters** setting and press the **[Enter]** key to confirm. Press numeric keys or rotate the knob to adjust the value in the current setting area. This value takes effect when you press **[Enter]**.

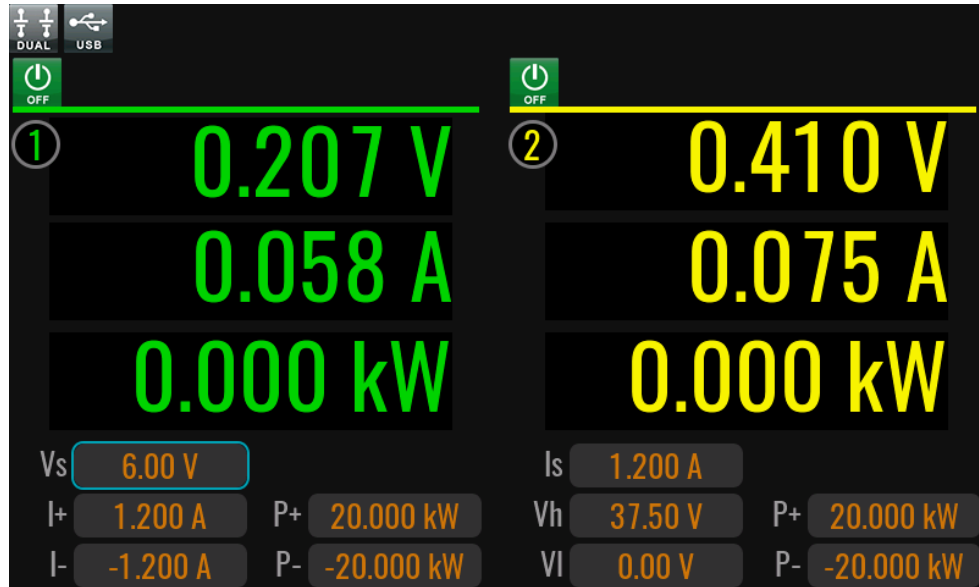


4.2.2 Set the Output Priority Mode

CV Priority

In CV priority mode, the output is controlled by a constant-voltage feedback loop, which maintains the output voltage at its programmed setting as long as the load current remains within the positive or negative current limit settings. CV priority mode is best suited for use with resistive or high impedance loads, and loads that are sensitive to voltage overshoots. Do not use CV priority mode with low-impedance sources such as batteries, power supplies, or large charged capacitors.

In CV priority mode, the output voltage should be programmed to the desired value. A positive and negative current limit value should also be set. The current limit should always be set to a value that is greater than the actual input current requirement of the external load. The following figure shows the CV priority operating locus of the output. The area in the white quadrants shows the output as a source (sourcing power). The area in the shaded quadrants shows the output as a load (sinking power).

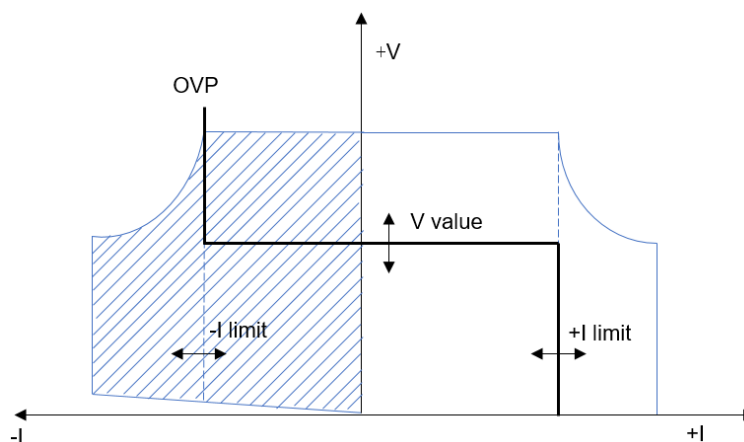

NOTE

In sink mode, there is a minimum operating voltage. The minimum operating voltage specification data corresponding to different voltage models are as follows.

| Voltage Level | Sink Current | Minimum Operating Voltage (MOV) | MOV/Vmax(%) |
|---------------|--------------|---------------------------------|-------------|
| 600V | -Imax | 3V | 0.5% |
| 1200V | -Imax | 6V | 0.5% |
| 800V | -Imax | 4V | 0.5% |
| 1600V | -Imax | 8V | 0.5% |
| 2250V | -Imax | 11.25V | 0.5% |

The heavy solid line illustrates the locus of possible operating points as a function of output. As shown by the horizontal portion of the line, the output voltage remains regulated at its programmed setting as long as the load current remains within the positive or negative current limit setting. A CV status flag indicates that the output voltage is being regulated and the output current is within its limit settings.


Note that when the output current reaches either the positive or negative current limit, the unit no longer operates in constant voltage mode and the output voltage is no longer held constant. Instead, the unit will now regulate the output current at its current limit setting.

As shown by the vertical portions of the shaded quadrants, the output voltage may continue to increase in the positive direction or decrease in the negative direction as current is forced into or pulled out of the unit. When the output voltage exceeds the over-voltage protection setting, the output will shut down.

CC Priority

In CC priority mode, the output is controlled by a bi-polar constant current feedback loop, which maintains the output source or sink current at its programmed setting. The output current remains at its programmed setting, provided the load voltage remains within the voltage limit setting. CC priority mode is best suited for use with batteries, power supplies, large charged capacitors, and loads that are sensitive to current overshoots. It minimizes current overshoots during programming, turn-on, and turn-off transitions and seamlessly transitions between positive and negative currents.

In CC priority mode, the output current should be programmed to the desired positive or negative value. A positive voltage limit range should also be set. The voltage upper limit should always be set to a value that is greater than the actual input voltage requirement of the external load. The following figure shows the CC priority operating locus of the output. The area in the white quadrants shows the output as a source (sourcing power). The area in the shaded quadrants shows the output as a load (sinking power).

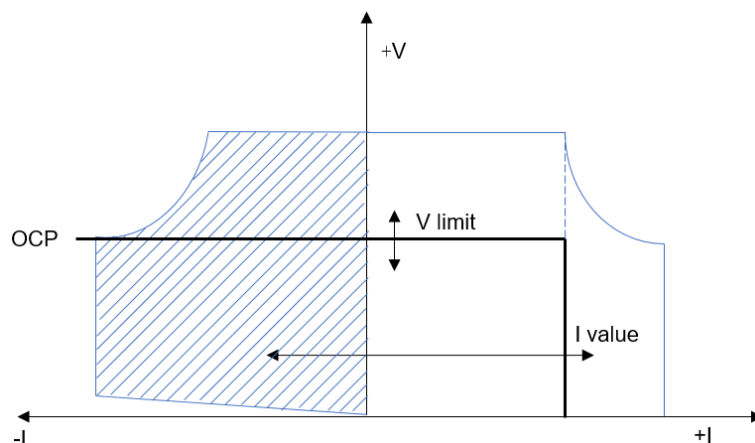


NOTE

In sink mode, there is a minimum operating voltage. The minimum operating voltage specification data corresponding to different voltage models are as follows.

| Voltage Level | Sink Current | Minimum Operating Voltage (MOV) | MOV/Vmax(%) |
|---------------|--------------|---------------------------------|-------------|
| 600V | -Imax | 3V | 0.5% |
| 1200V | -Imax | 6V | 0.5% |
| 800V | -Imax | 4V | 0.5% |
| 1600V | -Imax | 8V | 0.5% |
| 2250V | -Imax | 11.25V | 0.5% |

The heavy solid line illustrates the locus of possible operating points as a function of output. As shown by the vertical portion of the line, the output current remains regulated at its programmed setting as long as the output voltage remains within its limit setting. A CC (constant current) status flag indicates that the output current is being regulated and the output voltage is within its limit settings.

Note that when the output voltage reaches the upper limit, the unit no longer operates in constant current mode and the output current is no longer held constant. Instead, the unit will now regulate the output voltage at its voltage limit setting.

As shown by the horizontal portion of the shaded quadrants, when the unit is sinking power, the output current may continue to increase in the negative direction as more current is forced into the unit. This can happen when the instrument is connected to an external device such as a battery, and its output voltage is higher than the voltage limit setting of the instrument. Once the current exceeds the built-in negative over-current limit, the output will shut down. In such a case, it is important to set the voltage limit properly in order prevent this protection shutdown.

How to Set

The procedures to set the output priority mode are as follows.

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.
2. Press the up/down key or rotate the knob to find **Priority Mode** menu.
 - i. Press the up/down key to move the cursor to the Mode function setting and press the **[Enter]** key to confirm. Rotate the knob to set CC priority or CV priority, and press the **[Enter]** key to confirm.
 - ii. Press the up/down key to move the cursor to the **Loop Speed** function setting and press the **[Enter]** key to confirm. Use the numeric keys to set CC or CV loop response speed, and press the **[Enter]** key to confirm.
3. Press **[Esc]** to exit.

4.2.3 Set Output Slew

This series instrument is supported setting the V-Rise/V-Fall under CV priority mode and I-Rise/I-Fall under CC priority mode. The slew is the time for one voltage/current point to rise/fall to the other point under the output status is ON.

This series instrument offers two types of slew modes: time slew and standard slew. The standard slew is influenced by series and parallel connections. Please

refer to the table below for the relevant slew parameters.

| Slew | Priority mode | Unit | Minimum value | Maximum value (Num is the number of instruments connected in parallel or series.) | Default value |
|----------|---------------|------|---------------|---|-----------------|
| Time | CV | ms | 0.2ms | - | 100ms |
| | CC | ms | 0.2ms | - | 100ms |
| Standard | CV | V/ms | - | <ul style="list-style-type: none"> ● Parallel & Dual Channel: $V_{max}/0.2ms$ ● Series: $V_{max}/0.4ms$ | $V_{max}/100ms$ |
| | CC | A/ms | - | <ul style="list-style-type: none"> ● Parallel: $I_{max}/(0.4ms*Num)$ ● Series & Dual Channel: $I_{max}/(0.2ms*Num)$ | $I_{max}/100ms$ |

The instrument displays different slew parameters according to present CC or CV priority.

- When CV priority mode: displays V-Rise and V-Fall.
- When CC priority mode: displays I-Rise and I-Fall.

The following takes the CV priority mode as an example to introduce the operation of setting slew, the setting method under CC priority mode is the same.

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.
2. Press the up/down key or rotate the knob to find **Priority Mode** menu.
 - i. Press the up/down key to move the cursor to the Mode function setting and press the **[Enter]** key to confirm. Rotate the knob to select the CV priority and press the **[Enter]** key to confirm.
 - ii. Press the up/down key to move the cursor to the **Loop Speed** function setting and press the **[Enter]** key to confirm. Use left and right keys and knob to setting the CV loop response speed and press **[Enter]** to confirm.
3. Press the up/down key or rotate the knob to find **Slew Config** menu.
 - i. Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select the slew unit and press the **[Enter]** key to confirm.
 - ii. Press the up/down key to move the cursor to the **V-Rise** function setting and press the **[Enter]** key to confirm. Use left/right keys and knob to setting the voltage rise slew and press **[Enter]** to confirm.
 - iii. Press the up/down key to move the cursor to the **V-Fall** function setting and press the **[Enter]** key to confirm. Use left/right keys and knob to setting the voltage fall slew and press **[Enter]** to confirm.
4. Press **[Esc]** to exit.

4.2.4 Set the Internal Resistance

This series instrument provides internal resistance setting (CV priority mode only). The procedures are shown as below.

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.

2. Press the up/down key or rotate the knob to find **Output Resistance** menu.
 - i. Press the up/down key to move the cursor to the **Level** function setting and press the **[Enter]** key to confirm. Use the numeric keys to set the internal resistance value and press **[Enter]** to confirm.
3. Press **[Esc]** to exit.

4.2.5 Set the Output-On/Output-Off Delay

You can set the output-on/output-off delay time within the range from 0 seconds to 60 seconds.

- On Delay+Offset: Indicates from the time that a command to turn on the output is received until the output actually turns on.
- Off Delay+Offset: Indicates from the time that a command to turn off the output is received until the output actually turns off.

The procedures to set the output delay time are as follows.

1. Press the composite keys **[Shift] + [V-set]** (Config) on the front panel to enter the config menu.
2. Press the up/down key or rotate the knob to find **Onoff Delay** menu.
 - i. Press the up/down key to move the cursor to the **On Delay** function setting and press the **[Enter]** key to confirm. Use the numeric keys to set the on delay time and press the **[Enter]** key to confirm.
 - ii. Press the up/down key to move the cursor to the **Off Delay** function setting and press the **[Enter]** key to confirm. Use the numeric keys to set the off delay time and press the **[Enter]** key to confirm.
3. Press **[Esc]** to exit.

4.2.6 Enable the Output

User can control the output switching of the instrument's 2 channels by pressing the **[CH1 On/Off]** key and the **[CH2 On/Off]** key on the front panel. When receive the On/Off command, the instrument enable or disable the output according to the On/Off delay time. If the On/Off delay time set to 0, the source enable or disable output immediately. Detailed information of On/Off delay time refers to [4.2.5 Set the Output-On/Output-Off Delay](#).

- When **[On/Off]** key is lit, indicates the output is enabled, the LCD displays source present run mode.
- When **[On/Off]** key is lit, indicates the output is disabled, the LCD displays source state is OFF.

4.3 Protection Function

Press **[Shift]+[Recall]** (Protect) and enter to **Protect** configure menu, where you can set the following protection.

| | | |
|-------------------------|--------|---|
| Over Voltage Protection | OVP | |
| | Status | Configure over-voltage protection: On or Off. |
| | Level | OVP limit. |
| | Delay | Protection delay time. |
| Over Current Protection | OCP | |
| | Status | Configure over-current protection: On or Off. |
| | Level | OCP limit. |
| | Delay | Protection delay time. |

| | | |
|--------------------------|---------------------------------|--|
| Over Power Protection | OPP | |
| | Status | Configure over-power protection: On or Off. |
| | Level | OPP limit. |
| | Delay | Protection delay time. |
| Under Voltage Protection | UVP | |
| | Status | Configure under-voltage protection: On or Off. |
| | Warm up time | Indicates the instrument warm-up time. |
| | Level | UVP limit. |
| | Delay | Protection delay time. |
| Under Current Protection | UCP | |
| | Status | Configure under-current protection: On or Off. |
| | Warm up time | Indicates the instrument warm-up time. |
| | Level | UCP limit. |
| | Delay | Protection delay time. |
| Maximum Voltage Limit | Sets the maximum voltage value. | |
| | Level | The maximum voltage value. |
| Maximum Current Limit | Sets the maximum current value. | |
| | Output | The maximum output current value. |
| | Sink | The maximum input current value. |
| Maximum Power Limit | Sets the maximum power value. | |
| | Output | The maximum output power value. |
| | Sink | The maximum input power value. |

4.3.1 Over Voltage Protection

Over-voltage protection function allows the user to enable the protection and set a over-voltage limit (Level) and delay time (Delay). The function is mainly used to protect the DUT connected during test to prevent it from damage due to over-voltage.

How to Set

1. Press **[Shift]+[Recall]** (Protect) keys and enter to Protection menu.
2. Press the up/down key or rotate the knob to select Over Voltage Protection.
3. Set the protection status, protection Level and the delay time in sequence, and press **[Enter]** to confirm.

Clear OVP Protection

When OVP protection occurs, the instrument responds as follows:

- Instrument output is off.
- The instrument emits an alarm sound every 3 seconds.
- The main interface status bar displays the OVP icon.

To clear the OVP and return to normal operation, firstly remove the conditions that caused the protection fault. Press **[Shift] +[Esc]** keys (or send the command PROtection:CLEar) to clear the protection status. The message displayed in front panel is cleared and the instrument exits protection status.

4.3.2 Over Current protection

Over-current protection function allows the user to enable the protection and set

a over-current limit (Level) and delay time (Delay). The function is mainly used to protect the DUT connected during test to prevent it from damage due to over load.

How to Set

1. Press **[Shift]+[Recall]** (Protect) keys and enter to Protection menu.
2. Press the up/down key or rotate the knob to select Over Current Protection and press **[Enter]**.
3. Set the protection status, protection Level and the delay time in sequence, and press **[Enter]** to confirm.

Clear OCP Protection

When OCP protection occurs, the instrument responds as follows:

- Instrument output is off.
- The instrument emits an alarm sound every 3 seconds.
- The main interface status bar displays the OCP icon.

To clear the OCP and return to normal operation, firstly remove the conditions that caused the protection fault. Press **[Shift] +[Esc]** keys (or send the command PROTection:CLEAr) to clear the protection status. The message displayed in front panel is cleared and the instrument exits protection status.

4.3.2 Over Power protection

Over-power protection function allows the user to enable the protection and set a over-power limit (Level) and delay time (Delay). The function is mainly used to protect the DUT connected during test to prevent it from damage due to over load.

How to Set

1. Press **[Shift]+[Recall]** (Protect) keys and enter to Protection menu.
2. Press the up/down key or rotate the knob to select Over Power Protection and press **[Enter]**.
3. Set the protection status, protection Level and the delay time in sequence, and press **[Enter]** to confirm.

Clear OPP Protection

When OPP protection occurs, the instrument responds as follows:

- Instrument output is off.
- The instrument emits an alarm sound every 3 seconds.
- The main interface status bar displays the OPP icon.

To clear the OPP and return to normal operation, firstly remove the conditions that caused the protection fault. Press **[Shift] +[Esc]** keys (or send the command PROTection:CLEAr) to clear the protection status. The message displayed in front panel is cleared and the instrument exits protection status.

4.3.4 Under Voltage Protection

Users can enable the UVP function and set the instrument warm-up time (Warm up time), protection limit (Level) and protection delay time (Delay). When the voltage (i.e., the Meter value) is lower than this protection limit and the warm-up time, delay time are exceeded, the power supply will enter the UVP state.

How to Set

1. Press **[Shift]+[Recall]** (Protect) keys and enter to Protection menu.
2. Press the up/down key or rotate the knob to select Under Voltage Protection.
3. Set the protection status, warm up time, protection Level and the delay time in sequence, and press **[Enter]** to confirm.

Clear UVP Protection

When UVP protection occurs, the instrument responds as follows:

- Instrument output is off.
- The instrument emits an alarm sound every 3 seconds.
- The main interface status bar displays the UVP icon.

To clear the UVP and return to normal operation, firstly remove the conditions that caused the protection fault. Press **[Shift] +[Esc]** keys (or send the command PROTection:CLEar) to clear the protection status. The message displayed in front panel is cleared and the instrument exits protection status.

4.3.5 Under Current Protection

Users can enable the UCP function and set the instrument warm-up time (Warm up time), protection limit (Level) and protection delay time (Delay). When the current (i.e., the Meter value) is lower than this protection limit and the warm-up time, delay time are exceeded, the power supply will enter the UCP state.

How to Set

1. Press **[Shift]+[Recall]** (Protect) keys and enter to Protection menu.
2. Press the up/down key or rotate the knob to select Under Current Protection.
3. Set the protection status, warm up time, protection Level and the delay time in sequence, and press **[Enter]** to confirm.

Clear UCP Protection

When UCP protection occurs, the instrument responds as follows:

- Instrument output is off.
- The instrument emits an alarm sound every 3 seconds.
- The main interface status bar displays the UCP icon.

To clear the UCP and return to normal operation, firstly remove the conditions that caused the protection fault. Press **[Shift] +[Esc]** keys (or send the command PROTection:CLEar) to clear the protection status. The message displayed in front panel is cleared and the instrument exits protection status.

4.3.6 Set Maximum Voltage/Current/Power Limit

The voltage output can be adjusted between 1% and 100% of V_{max} , while the current output and power output can be adjusted between 0% and 100%. You can set upper limits for the output voltage, current, and power in the Protection menu.

Limit factory setting is the rated output voltage/current/power of corresponding model of the power supply.

Take the voltage limit setting for an example, the operating as follows:

1. Press **[Shift]+[Recall]** (Protect) keys and enter to Protection menu.
2. Press the up/down key or rotate the knob to select Maximum Voltage Limit

and press **[Enter]**.

3. Set the maximum Voltage limit, and press **[Enter]** to confirm.

4.3.7 Over-temperature protection (OTP)

When the temperature of the power component in the power supply exceeds 95°C, the temperature protection will be enabled. In this case, the power supply will be automatically OFF, and the LCD will display OTP icon. At the same time, the OT position in the status register will be set and kept until power supply is reset.


Clearing over-temperature protection:

When the power supply temperature decreases to the protection temperature, press **[Shift]+[Esc]** keys on the front panel (or send the command "PROTection:CLEar"). Then OTP on the power supply screen will disappear, and the power supply will exit the OTP status.

4.3.8 Sense Reverse Protection

The instrument defaults to provide sense reverse protection. The premise is that the Sense switch is turned on. When the output state is ON and the difference between output terminal voltage and sense remote voltage exceeds the sense compensation voltage, sense reverse protection will be enabled after 500ms. The power supply output will be immediately switched to Off and the buzzer will




sound if the sense terminals are reversed. The display screen will display . Press **[Shift]+[Esc]** keys (or send the command "PROTection:CLEar") to clean the protection.

When the power source is in Sense Reverse Protection state, you should check the whether the polarities are connected reversely or not firstly. When the polarities connect correctly, please press **[On/Off]** button. Then the unit could have a output voltage again.

4.4 LIST Function

The user can edit the test procedure composed of several steps with the List function. With List function, a maximum of 100000 steps can be configured for each List file. The user needs to edit the voltage/current value, slope and duration of each step, and set certain repeated number of times and final state for each List file. After the file is edited completely, you can trigger the selected List file to run according to the selected trigger mode.

Introduction of List interface

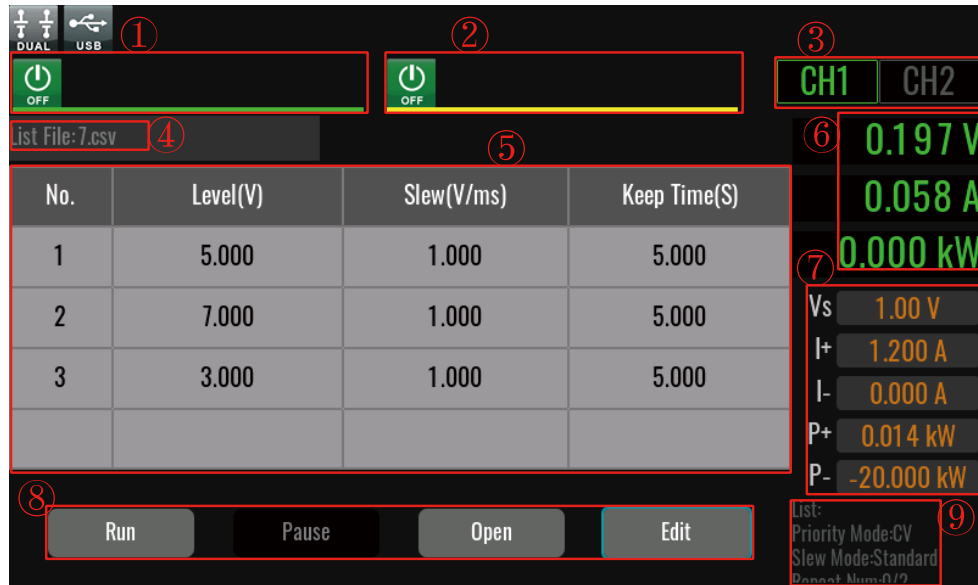


1. CH1 status bar: displays the output status of power channel 1.
2. CH2 status bar: displays the output status of power channel 2.
3. CH1/CH2: channel selection, Channel 1 or Channel 2.
4. 7.csv: the list file name to execute.
5. List display area: this area mainly displays the edited List, you can view this list by sliding up and down.
6. Output values view area: displays the output voltage value, output current value and output power value of the current channel.
7. Setting values view area (Normal mode): When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.
8. List edit button. The functions are described as follows.
 - Run/Stop: run/stop the list function.
 - Pause: suspend list running. Resume: continue to run the list.
 - Open: select the List file to execute.
 - Edit: edit present list file.
9. Displays the List function relevant parameters, which can be viewed by sliding up and down.
 - Priority Mode: list running priority mode.
 - Slew Mode: slew unit.
 - Repeat Num: X/Y, X indicates the current number of cycles and Y indicates the total number of cycles.
 - Tout: trigger output setting.
 - End Mode: end state setting.
 - Current Step: A/B, A indicates the number of current running steps and B indicates the total number of steps.

- RunState
- RunTime

Edit List files

The following takes CV priority mode as an example to introduce the operation of editing three test steps.

1. Press **[Shift]+[I-set]**(List) on the front panel to enter the List function main interface.
2. Click the **[Edit]** key on the screen and enter to the List file edit interface.



| No. | Level(V) | Slew(V/ms) | Keep Time(S) |
|------|----------|------------|--------------|
| 1... | 5.00 | 1.000 | 5.000 |
| 2... | 7.00 | 1.000 | 5.000 |
| 3... | 3.00 | 1.000 | 5.000 |
| 4 | | | |

List parameters description:

| Parameter | Description |
|---|--|
| Description | Description of List, display list file name. |
| Edit the attribute parameters of List file. | |
| Priority Mode | List running priority mode. |
| Repeat | Edit the cycles of the List file. You can choose Infinite and Count, when you choose Count, you also need to set the total number of loops, set the range: 1-9999999. |
| Trig out | Function switch that triggers the signal output. <ul style="list-style-type: none"> ● Off: Turn off. ● On: Turn on. When IO-4 is configured as Trigger-out, a pulse signal will be output from IO-4 when triggering the List function. |
| Slew Mode | Select the slew unit. <ul style="list-style-type: none"> ● Time: describe the slew of the device in terms of time. ● Standard: standard slew, unit is V/ms or A/ms. |
| End Mode | Set the final waveform, with the following options available: <ul style="list-style-type: none"> ● Off: directly off the output after operation. ● Normal: return to normal after operation. ● Last: keep the last waveform output unchanged after operation. |

| | |
|--|--|
| Trig Source | Select the trigger source for running this list file. <ul style="list-style-type: none"> ● Immediate: Perform a trigger operation immediately. ● Manual: Indicates the trigger occurs when the [Shift]+[5](Trigger) keys are pressed from the front panel. ● Bus: Bus trigger. When the trigger command *TRG is received, the instrument generates a trigger. ● External: Indicates the trigger occurs via the pin 4 of the digital I/O interface (P-IO). For details, see 5.9 Digital I/O Function. |
| Edit the step parameters of List file. | |
| No. | Step number of list. Click the number, you can operate such as copy/paste/cut/insert/delete. |
| Level | Voltage value/current value. |
| Slew | Slew value. |
| Keep Time | Width time. The range is from 0.001 to 21000 in seconds. |
| | |
| Save | Save the list file. |
| Config | Configure the list file to make it effective. |
| Clear all | Delete all of step information. |

- Fill in corresponding parameter in the List file edit interface and press **[Save]**.
At list Edit interface, click the step number, the **[Copy]/[Paste]/[Cut]/[Insert]/[Delete]** will display, click the key to edit.
- Press **[Esc]**, and return to the List function interface. The List display zone displays the edited List file.

Select/Run List File

If several List files are edited, press **Open** to recall the List file to be tested. Detailed operation steps are as below:

- Press **[Shift]+[I-set]**(list) on the front panel to enter the List function main interface.
- Click the **[Open]** key on the screen, select the saved 7.csv file, and click the **[Open]** key to enter the file.
- Press **[On/Off]** on the front panel, turn on the output.
- Press **[Run]** key in the list function interface.
- Based on the selected trigger method, perform the trigger operation.

Take the manual trigger as an example. Press **[Shift]+[5]**(Trigger) on the front panel to run the selected List file.

Stop Running the List Program

When the List program is running, if you click **Stop**, it means to stop the present running, and you can wait for the next trigger to run; if you click **Pause**, it means that the present running is suspended, and you can continue to run by click **Resume**.

Import/Export List file

- **Import List file**

IT6600 series support import list file function, the user can finish the editing of List file in Excel and import it into the software. This function simplifies the List file edit and facilitates user operation.


To help user define an Excel file format, please export a CSV template from the List interface.

Detailed operation steps are as below:

1. Create a new Excel document on local PC and name it 5.csv.
2. Open the Excel document and save it as in “other formats” i.e. “(*.csv)”.
3. Open the 5.csv document and edit the List. Set every step of the List and corresponding parameters and save the document in the USB disk.

| | A | B | C | D | E |
|----|-------------|----------|------------|--------------|---|
| 1 | Model | IT6600 | | | |
| 2 | Version | 123 | | | |
| 3 | File Type | List | | | |
| 4 | Priority | McCV | | | |
| 5 | Repeat | McCount | | | |
| 6 | Repeat Co | 2 | | | |
| 7 | End | OFF | | | |
| 8 | Slew Mode | Standard | | | |
| 9 | Trig Source | Manual | | | |
| 10 | Trig Out | OFF | | | |
| 11 | Step total | 3 | | | |
| 12 | Step Index | Level(V) | Slew(V/ms) | Keep Time(S) | |
| 13 | 1 | 5 | 1 | 5 | |
| 14 | 2 | 7 | 1 | 5 | |
| 15 | 3 | 3 | 1 | 5 | |
| 16 | | | | | |

- The list files for dual-channel output mode and parallel output mode need to be placed in the listParallel folder of the USB flash drive.
- The list file for serial output mode needs to be placed in the listSeries folder on the USB flash drive.



4. Insert the USB disk into the USB interface of the front panel. Press **[Shift]+[I-set]**(List) on the front panel to enter the List function main interface.
5. Click the **[Open]** key on the screen, enter to list recall interface.
6. Click usb, select the 5.csv file in the usb, and click **[Open]** to confirm. The list file will be imported and the configured 5.csv file will appear in the interface.

- **Export List file**

After editing the List file, the user can directly save it into the device or export and save it into the peripheral memory disc. The exported List is saved in the format of. (*.csv). Detailed operation steps are as below:

1. Insert the U disk into the USB interface of the front panel. (The USB type needs to be set as Host.)
2. Press **[Shift]+[I-set]**(List) on the front panel to enter the List function

main interface.

3. Click the [**Edit**] key on the screen, enter to list file edit interface.
4. Click the [**Save**] key to enter the list save interface.
5. Click usb, set the FileName of the exported file, and click [**Save**] to confirm the export. Then you can export the list file from Edit interface to USB disk.

4.4.1 ARB Function

This series of instruments comes standard with ARB (arbitrary waveform) function, which allows the output of user-defined arbitrary complex voltage or current waveforms. It can be operated in the following ways:

Import via U disk

The instrument supports importing the edited .csv format file (the template can be obtained by contacting ITECH personnel) through the USB interface on the front panel, and generating voltage or current values after parsing, and then outputting complex voltage or current waveforms according to the time width specified by the user. The user can edit a .csv file containing up to 80 million voltage or current points and import it into the instrument for running to realize arbitrary waveform output or working condition simulation.

The instrument has the ability to quickly parse data. A .csv file of dozens of megabytes can be imported and parsed within 5S, making testing more convenient and efficient.

This instrument supports importing the .csv files corresponding to the following waveforms:

- **CDWELL: Constant dwell arbitrary waveform**

The fields included in the .csv template file are explained as follows:

| | |
|------------------|---|
| Model | Device model, keep the default settings without modification. |
| Firmware Version | Firmware version number, keep the default settings without modification. |
| Serial Number | Device serial number, keep the default settings without modification. |
| File Type | File type, keep the default settings without modification. |
| Waveform Type | Waveform type, keep the default settings without modification. |
| Value Unit | The CV priority is set to V, and the CC priority is set to A. |
| Offset Unit | Offset value unit, CV priority is set to V, CC priority is set to A. |
| Time Unit | Time unit, fixed to S. |
| Mode | Indicates the power supply working mode. The CV priority is set to CV, and the CC priority is set to CC. |
| Repeat | Repeat times, the setting range is 1~65535. |
| End State | Indicates the end state. Last (voltage or current maintained at the last point after completion) or Normal (return to the mode before CDWELL execution after completion). |
| Total Point | The total number of waveform points. |
| Keep Time | Indicates the pulse width of each point. Range: 0~3600. Unit: seconds. |
| Value | Voltage or current value at each point. |

- List: User-defined waveform

The fields included in the .csv template file are explained as follows:

| | |
|------------------|---|
| Model | Device model, keep the default settings without modification. |
| Firmware Version | Firmware version number, keep the default settings without modification. |
| Serial Number | Device serial number, keep the default settings without modification. |
| File Type | File type, keep the default settings without modification. |
| Waveform Type | Waveform type, keep the default settings without modification. |
| Value Unit | The CV priority is set to V, and the CC priority is set to A. |
| Slope Unit | Slope unit, fixed to S. |
| Time Unit | Time unit, fixed to S. |
| Mode | Indicates the power supply working mode. The CV priority is set to CV, and the CC priority is set to CC. |
| Step Count | The total number of steps, up to 10 million points can be edited. |
| Repeat | Repeat times, the setting range is 1~65535. |
| End State | Indicates the end state. Last (the voltage or current maintained at the last step after the end) or Normal (return to the normal mode before the List is executed after the end). |
| Step Index | The sequence number of the single step. |
| value | Voltage or current value for a single step. |
| slope | Slope for a single step. |
| Keep Time | Pulse width for a single step. |

- Sine: Sine wave

The fields included in the .csv template file are explained as follows:

| | |
|------------------|--|
| Model | Device model, keep the default settings without modification. |
| Firmware Version | Firmware version number, keep the default settings without modification. |
| Serial Number | Device serial number, keep the default settings without modification. |
| File Type | File type, keep the default settings without modification. |
| Waveform Type | Waveform type, keep the default settings without modification. |
| Amp Unit | Peak-to-peak unit, CV priority is set to V, CC priority is set to A. |
| Offset Unit | Offset value unit, CV priority is set to V, CC priority is set to A. |
| Frequency Unit | Frequency unit, Hz. |
| Mode | Indicates the power supply working mode. The CV priority is set to CV, and the CC priority is set to CC. |
| Repeat | Repeat times, the setting range is 1~65535. |
| Amp | Peak-to-peak |
| Offset | Offset value |
| Frequency | Frequency value, the default maximum is 250Hz. |

| | |
|-----------|--|
| End State | Indicates the end state. Last (the voltage or current maintained at the last step after the end) or Normal (returns to the normal mode before Sine is executed). |
|-----------|--|

- **Sweep: Sweep wave**


The fields included in the .csv template file are explained as follows:

| | |
|------------------|--|
| Model | Device model, keep the default settings without modification. |
| Firmware Version | Firmware version number, keep the default settings without modification. |
| Serial Number | Device serial number, keep the default settings without modification. |
| File Type | File type, keep the default settings without modification. |
| Waveform Type | Waveform type, keep the default settings without modification. |
| Amp Unit | Peak-to-peak unit, CV priority is set to V, CC priority is set to A. |
| Offset Unit | Offset value unit, CV priority is set to V, CC priority is set to A. |
| Time Unit | Time unit, S. |
| Frequency Unit | Frequency unit, Hz. |
| Mode | Indicates the power supply working mode. The CV priority is set to CV, and the CC priority is set to CC. |
| Repeat | Repeat times, the setting range is 1~65535. |
| Amp | Peak-to-peak |
| Offset | Offset value |
| Start Frequency | Start frequency |
| End Frequency | Stop frequency |
| Step DwellH | Total running time. |
| Step time | Single-step pulse width. Single-step pulse width and single-step repetition times can be set by selecting one of them. |
| Step Repeat | The number of repetitions of a single step. Singlestep pulse width and single-step repetition times can be set by selecting one of them. |
| Step mode | Operation mode, can be set to 0 or 1. When set to 0, it means that the total running time Step DwellH and the single-step pulse width Step time are used as the running end condition; when set to 1, it means that the single-step repetition times Step Repeat is used as the running end condition. |
| End State | Indicates the end state. Last (the voltage or current maintained at the last step after the end) or Normal (return to the normal mode before the Sweep is executed). |

The steps are as follows:

1. Edit the 8.csv file corresponding to the template on the PC and save it.
2. Save the edited file in the U disk.
 - The ARB files for dual-channel output mode and parallel output mode need to be placed in the arbParallel folder of the USB flash drive.
 - The ARB file for serial output mode needs to be placed in the arbSeries

folder on the USB flash drive.



3. Insert the U disk into the front panel of the instrument. (The USB type needs to be set as Host.)
4. Click ARB on the Menu screen to enter the ARB function main interface.
5. Click the **[Open]** key on the screen, enter to ARB recall interface.
6. Click usb, select the 8.csv file in the usb, and click **[Open]** to confirm. The ARB file will be imported.
7. Press **[On/Off]** on the front panel, turn on the output.
8. Press **[Run]** key in the ARB function interface.
9. Based on the selected trigger method, perform the trigger operation.
 Take the manual trigger as an example. Press **[Shift]+[5]**(Trigger) on the front panel to run the selected ARB file.

Programming via SCPI instructions

For detailed instructions and parameter introduction, please refer to the instructions of "ARB Subsystem" in the Programming Guide.

Realized by the software PV6600 on PC

For detailed function usage, please refer to PV6600 User Manual.

4.5 Battery Charging/Discharging Test Function


This series power supply provides the battery charging/discharging test function based on its unique bidirectional power supply properties. Suitable for charging/discharging tests on all types of portable batteries.

WARNING

- When connecting the DUT (battery/capacitor), do not short-circuit the battery/capacitor.
- It is recommended that for battery testing, a fuse must be connected in series between the power supply and the battery to prevent short circuits caused by any problems.
- When connecting the DUT (including but not limited to battery/capacitor), it is recommended that you purchase the IT-E165A anti-reverse connection and anti-spark module to prevent the battery/capacitor reverse connection that may cause damage to the instrument and spark during the battery/capacitor wiring; When there is no external auxiliary equipment connected to prevent reverse connection and anti-spark function, please pay attention to the safety of the wiring, and be careful not to reverse the battery/capacitor connection, reverse connection will cause damage to the instrument, even if it is not powered on.
- Before performing the battery test, you need to connect the Sense cables to both ends of the battery. If the Sense cables are not connected, the instrument cannot detect the Sense voltage and prompt "Wait Sense Link!", which will prevent the battery test from continuing.

Battery Charging Function

1. Click BAT on the Menu screen to enter the battery charging/discharging function interface.
2. Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Charge** and press the **[Enter]** key to confirm.

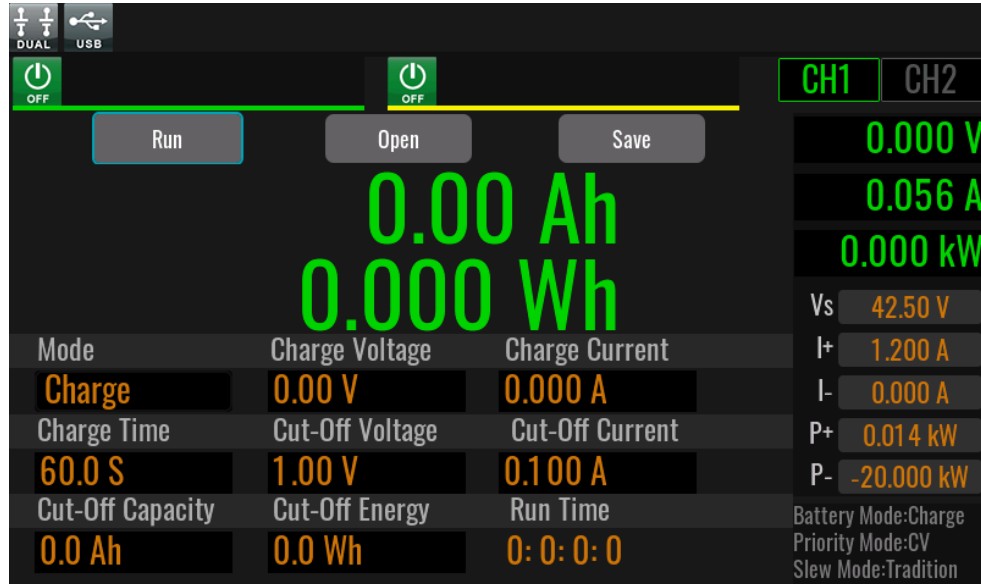


| Parameter | Description |
|------------------|--|
| Mode | Select mode: Charge (battery charge mode), Discharge (battery discharge mode). |
| Charge Voltage | Set the voltage value for charging. |
| Charge Current | Set the current value for charging. |
| Charge Time | Set the time value for charging. |
| Cut-Off Voltage | Battery test cut-off voltage. |
| Cut-Off Current | Battery test cut-off current. |
| Cut-Off Capacity | Battery test cut-off capacity. |
| Cut-Off Energy | Battery test cut-off energy. |
| Run Time | Display the running time of the battery test. |
| Run/Stop | Run/stop the Battery function. |
| Open | Select the Battery file to execute. |
| Save | Save the Battery file. |

3. Set the charging parameters for the battery and press the **[Save]** button to save.
4. Press **[On/Off]** on the front panel, turn on the output.
5. Press **[Run]** in the Battery function interface.
6. Press **[Shift]+[5]**(Trigger) on the front panel to run the battery charging test.
7. Click **[Stop]** to stop the present running.

Battery Discharging Function

1. Click BAT on the Menu screen to enter the battery charging/discharging function interface.

- Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Discharge** and press the **[Enter]** key to confirm.

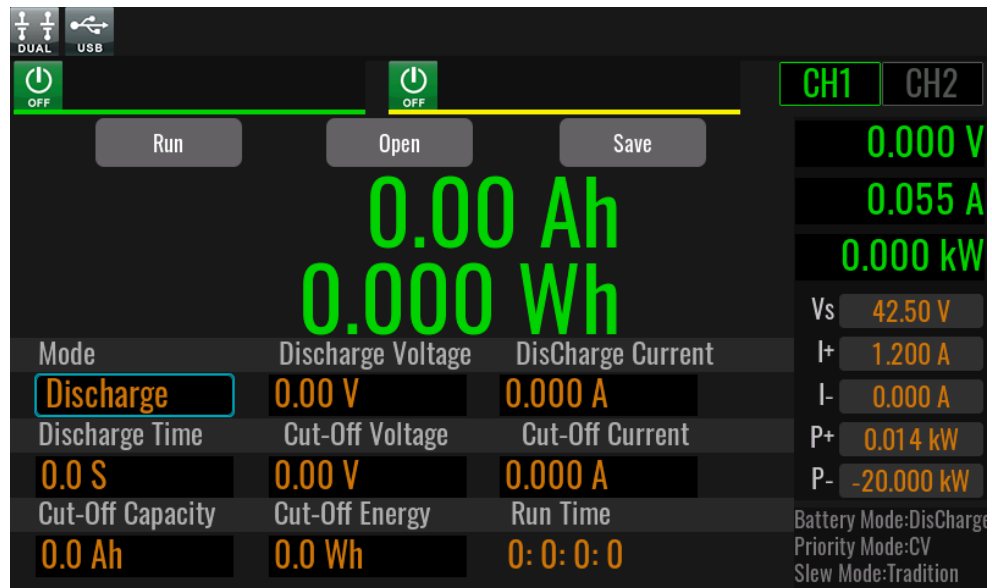

| Parameter | Description |
|-------------------|--|
| Mode | Select mode: Charge (battery charge mode), Discharge (battery discharge mode). |
| Discharge Voltage | Set the voltage value for discharging. |
| Discharge Current | Set the current value for discharging. |
| Discharge Time | Set the time value for discharging. |
| Cut-Off Voltage | Battery test cut-off voltage. |
| Cut-Off Current | Battery test cut-off current. |
| Cut-Off Capacity | Battery test cut-off capacity. |
| Cut-Off Energy | Battery test cut-off energy. |
| Run Time | Display the running time of the battery test. |
| Run/Stop | Run/stop the Battery function. |
| Open | Select the Battery file to execute. |
| Save | Save the Battery file. |


- Set the discharging parameters for the battery and press the **[Save]** button to save.
- Press **[On/Off]** on the front panel, turn on the output.
- Press **[Run]** in the Battery function interface.
- Press **[Shift]+[5]**(Trigger) on the front panel to run the battery discharging test.
- Click **[Stop]** to stop the present running.

4.6 Battery Simulation Function

The IT6600 series power supply can simulate battery characteristics in practical applications based on its unique bidirectional properties and the variable output impedance. You can set battery-related parameters to simulate the charge and discharge characteristics of the battery to assist with other tests.


Introduction of Battery Simulation interface

- Userdefined

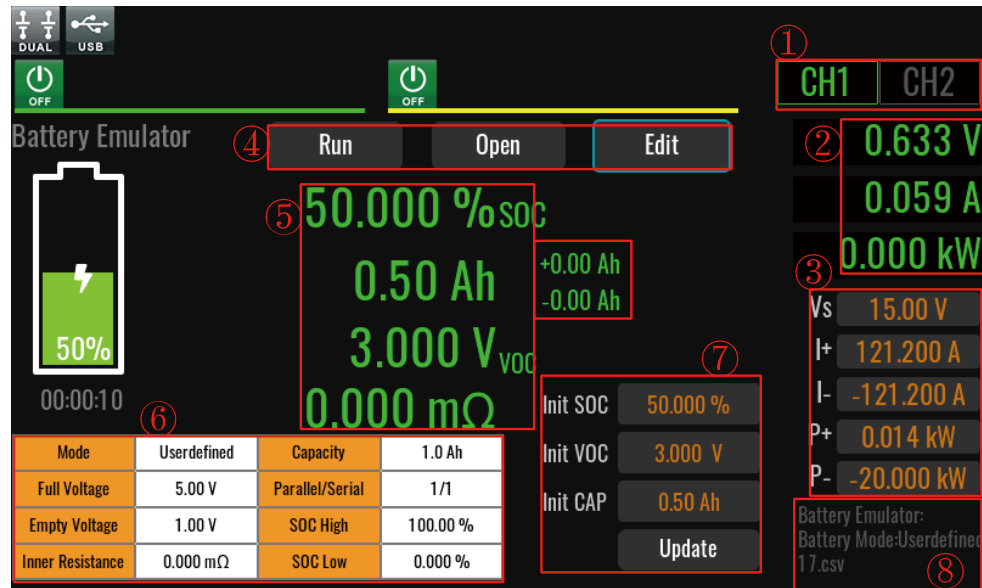

1. CH1/CH2: channel selection, Channel 1 or Channel 2.
2. Output values view area: displays the output voltage value, output current value and output power value of the current channel.
3. Setting values view area (Normal mode): When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.
4. Bat-SIM edit button. The functions are described as follows.
 - Run/Stop: run/stop the Bat-SIM function.
 - Open: select the Bat-SIM file to execute.
 - Edit: edit present Bat-SIM file.
5. Display the state of charge (Soc), capacity, open circuit voltage (Voc), and internal resistance of the current simulated battery.
+0.00Ah and -0.00Ah: These indicate the added and subtracted capacity during the simulated battery testing process.
6. Display the current edited battery simulation file parameters.
7. Quick edit area displays the initial state of charge (Init Soc), initial open circuit voltage (Init Voc), and initial capacity (Init CAP) for the current simulated battery. Click **[Update]** to confirm any modifications.
8. Displays the certain status information during Bat-SIM operation, which can be viewed by sliding up and down.

- Curve

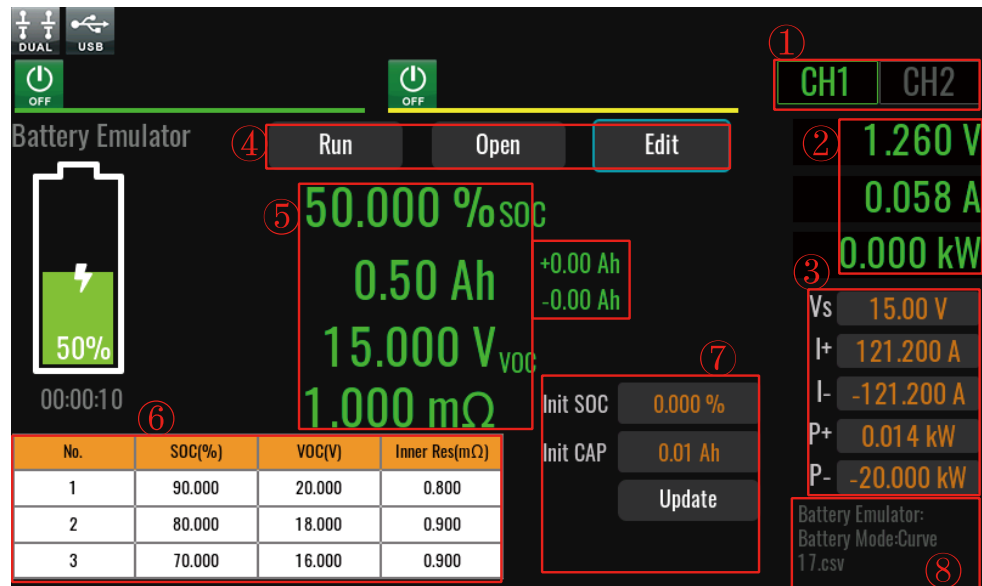

1. CH1/CH2: channel selection, Channel 1 or Channel 2.
2. Output values view area: displays the output voltage value, output current value and output power value of the current channel.
3. Setting values view area (Normal mode): When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.
4. Bat-SIM edit button. The functions are described as follows.
 - Run/Stop: run/stop the Bat-SIM function.
 - Open: select the Bat-SIM file to execute.
 - Edit: edit present Bat-SIM file.
5. Display the state of charge (Soc), capacity, open circuit voltage (Voc), and internal resistance of the current simulated battery.
+0.00Ah and -0.00Ah: These indicate the added and subtracted capacity during the simulated battery testing process.
6. Display the current edited battery simulation file parameters.
7. Display the initial state of charge (SoC) and initial capacity of the simulated battery. After making changes, please click [**Update**] to confirm.
8. Displays the Bat-SIM file attribute parameters, which can be viewed by sliding up and down.

Edit Battery Simulation Test File

- **Edit userdefined battery simulation file**
 1. Click **Battery Emulator** on the Menu screen to enter the Bat-SIM function main interface.
 2. Press [**Edit**] and enter to the Bat-SIM file edit interface.

Bat-SIM
CH1

File Name: No File Opened

Mode: Userdefined Save Config Esc

Single Cell Settings

Capacity 1.00 Ah Capacity of a single battery, range is [0.01, 9999.99], Def=1.00 Ah

Full Volt 5.00 V Voltage at full capacity, range is [0.00, 606.00], Def=5.00 V Empty Volt 1.00 V Voltage at empty capacity, range is [0.00, 606.00], Def=1.00 V

Battery Pack Settings

Serial Number 1 Serial quantity, range is [1, 99], Def=1 Parallel Number 1 Parallel quantity, range is [1, 99], Def=1

Inner Resistance 0.0000 mΩ Total internal resistance of the pack, range is [0.0000, 1.0000], Def=0.0000 mΩ

Protection Settings

Soc High: 100.000 % Upper limit of charging soc. Soc Low: 0.000 % Lower limit of discharge soc.

Bat-SIM edit description:

| Parameter | Description |
|-----------------------|--|
| File Name | Display Bat-SIM file name. |
| Mode | Select the Bat-SIM working mode Userdefined or Curve. |
| Save | Save the Bat-SIM file. |
| Config | Configure the Bat-SIM file to make it effective. |
| Single Cell Settings | Sets the properties of a single cell. <ul style="list-style-type: none"> ● Capacity: Simulates the capacity of a cell battery. ● Full Volt: Simulates the voltage value when the cell battery is fully charged. ● Empty Volt: Simulates the voltage value when the cell battery is in the empty state. |
| Battery Pack Settings | Sets the properties of battery pack. <ul style="list-style-type: none"> ● Serial Number: Set the number of parallel connected batteries. ● Parallel Number: Set the number of batteries in series. ● Inner Resistance: Simulates the total internal resistance of battery pack. |
| Protection Settings | <ul style="list-style-type: none"> ● Soc High: Upper limit of charge soc. ● Soc Low: Lower limit of discharge soc. ● Charge Curr Max: Upper limit of charge current. ● Discharge Curr Max: Lower limit of discharge current. |
| Running Settings | <ul style="list-style-type: none"> ● Init Soc: Set the initial state of charge (Soc) of the battery. 0~100% corresponds to the voltage range from no-load voltage to full-load voltage. ● Init Voc: Sets the initial battery open circuit voltage. ● Init Cap: Set the initial battery capacity. ● End Mode: Set the running state after the Bat-SIM execution is finished. <p>Last: Maintains the final voltage output after the end of charge or discharge.</p> <p>Normal: The device shuts down output and returns to normal.</p> |

3. Fill in corresponding parameter in the Bat-SIM edit interface, Press

[Save].

4. Press [Esc] to return and the interface appears with the edited Bat-SIM file.

- **Edit battery simulation curve file**

1. Click **Battery Emulator** on the Menu screen to enter the Bat-SIM function main interface.
2. Press [Edit] and enter to the Bat-SIM file edit interface.



| No | SOC (%) | VOC (V) | Inner Res (mΩ) |
|----|---------|---------|----------------|
| 1 | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |
| | | | |

Bat-SIM edit description:

| Parameter | Description |
|-----------|---|
| File Name | Display Bat-SIM file name. |
| Mode | Select the Bat-SIM working mode Userdefined or Curve. |
| Save | Save the Bat-SIM file. |
| Config | Configure the Bat-SIM file to make it effective. |
| More | More configurations. |
| Clear | Clear the battery characteristic data under editing. |
| SOC(%) | The capacity in percentage. |
| VOC | The open-circuit voltage of the battery. |
| Inner Res | The battery resistance. |

The introduction of More interface parameters is as follows:

| Parameter | Description |
|----------------------|--|
| Single Cell Settings | Sets the properties of a single cell. <ul style="list-style-type: none"> ● Capacity: Simulates the capacity of a cell battery. |
| Protection Settings | <ul style="list-style-type: none"> ● Soc High: Upper limit of charge soc. ● Soc Low: Lower limit of discharge soc. ● Charge Curr Max: Upper limit of charge current. ● Discharge Curr Max: Lower limit of discharge current. |

| Parameter | Description |
|------------------|--|
| Running Settings | <ul style="list-style-type: none"> ● Init Soc: Set the initial state of charge (Soc) of the battery. 0~100% corresponds to the voltage range from no-load voltage to full-load voltage. ● Init Cap: Set the initial battery capacity. ● End Mode: Set the running state after the Bat-SIM execution is finished. <p>Last: Maintains the final voltage output after the end of charge or discharge.</p> <p>Normal: The device shuts down output and returns to normal.</p> <p>Last+Off: After the charge and discharge process is completed, retain the final parameter settings and turn off the output.</p> |

3. Fill in corresponding parameter in the Bat-SIM edit interface. Click **[More]** enter to advanced menu of Bat-SIM file.
4. Press **[Esc]** to return Edit interface, Press **[Save]**.
5. Press **[Esc]** to return and the interface appears with the edited Bat-SIM file.

Select/Run Bat-SIM File

1. Click **Battery Emulator** on the Menu screen to enter the Bat-SIM function main interface.
2. Press **[Open]**, select the saved Bat-SIM01 csv file, and press **[Enter]** to enter the file.
3. Set Init Soc, Init Cap, Init Voc (only required for Userdefined mode), and press the **[Update]** button.
4. Press **[On/Off]** on the front panel, turn on the output.
5. Press **[Run]** in the Bat-SIM function interface.
6. Press **[Shift]+[5]**(Trigger) on the front panel to run the Bat-SIM test.
7. Click **[Stop]** to stop the present running.



NOTE

The battery simulation function is only available when the loop speed is set to medium or low. It cannot operate at high speed.

4.7 Built-in Waveform Function

This series power supply supports built-in waveforms for user to execute the test directly. The protocols/standards involved in the built-in waveforms include the following:

- DIN40839
- ISO16750-2
- ISO21848
- SAEJ1113-11
- LV123
- LV124
- LV148
- ISO21780
- ISO21498-2


4.7.1 DIN40839

This series power supply has built-in 12V or 24V DIN40839 waveform. This test verifies the behavior of a DUT during and after cranking. This waveform can reproduce the voltage curve for automotive power network confirms to DIN40839 standard, thus facilitating quick call by customers.

For automotive startup voltage waveform, the startup voltage can also be set based on customers' requirements. In this way, the user can create waveform between 8V to 32V.


DIN40839 for 12V System

| Step | Voltage(V) | Current(A) | Width(ms) | Slope(ms) |
|------|------------|------------|-----------|-----------|
| 1 | 4.5 | 60 | 15 | 5 |
| 2 | 6 | 60 | 2000 | 5 |
| 3 | 12 | 60 | T | 10 |

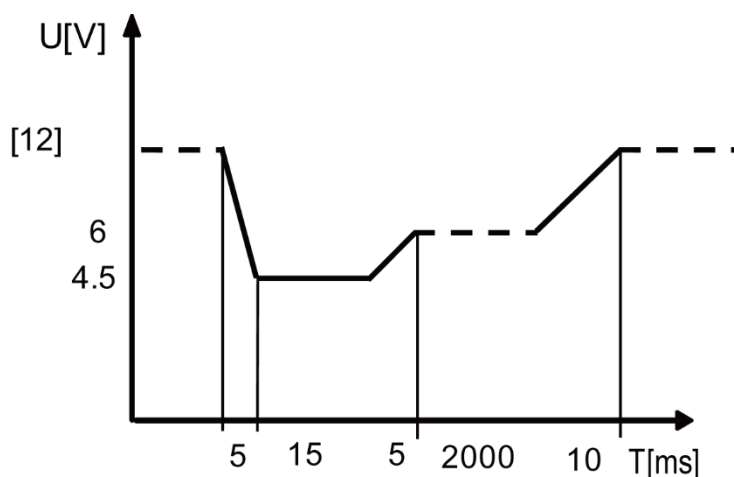

DIN40839 for 24V System


| Step | Voltage(V) | Current(A) | Width(ms) | Slope(ms) |
|------|------------|------------|-----------|-----------|
| 1 | 8 | 60 | 15 | 10 |
| 2 | 12 | 60 | 2000 | 5 |
| 3 | 24 | 60 | T | 10 |

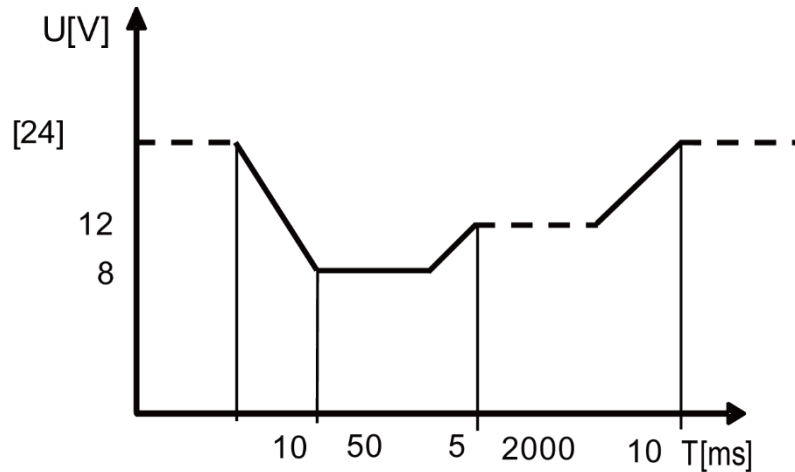


User-defined Startup Voltage Waveform System

The user can define the startup voltage, ranging from 8V to 32V. When the waveform program is divided into 8V-16V, the waveform is consistent with standard 12V; when the waveform program is divided into 16V-32V, the waveform is consistent with the standard 24V waveform. The waveform diagram is shown below.

- **8V~16V**

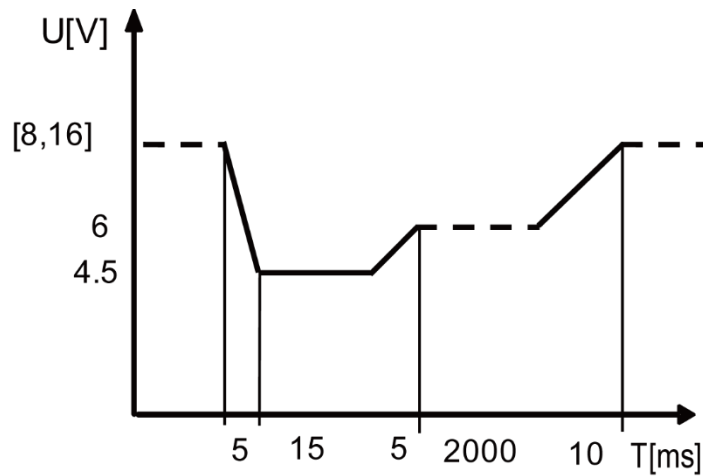

- **16V~32V**

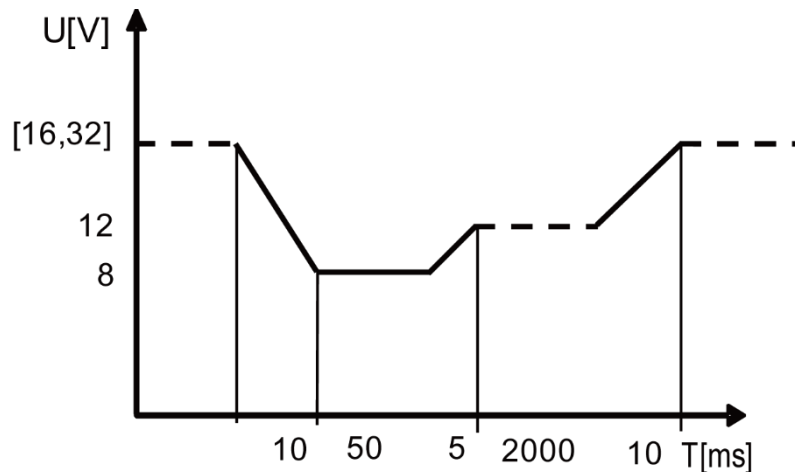

How to Use

Recall the self-defined DIN waveform operation (taking 12.5V voltage waveform as an example):

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **DIN40839** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Userdefined** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Voltage** function setting and press the **[Enter]** key to confirm. Press the numeric keys to set the startup voltage as V=12.5V and press **[Enter]** to confirm.
2. Press **[On/Off]** on the front panel, turn on the output.
3. Press **[Run]** in the Vehicle function interface to output the startup voltage waveform.


4.7.2 ISO16750-2

To verify the anti-interference performance of the automotive electronics' products. Output pulse waveform completely meets the International Standard ISO-16750-2, convenient for quick recall by the user.


Automotive Short-time Voltage Drop Waveform

This waveform simulates an instantaneous drop in the supply voltage when the car is started. This test simulates the effect when a conventional fuse element melts in another circuit.

- 12V system

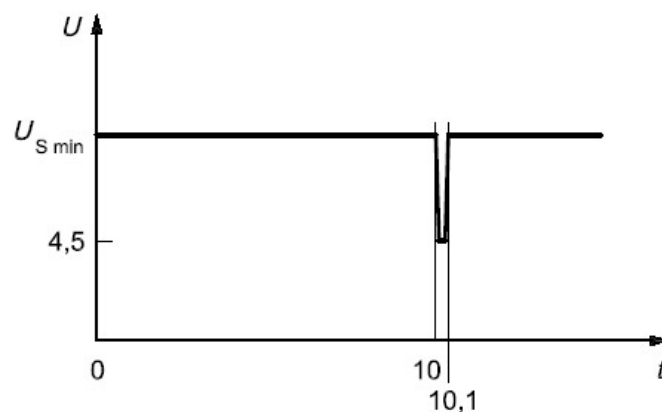

- 24V system

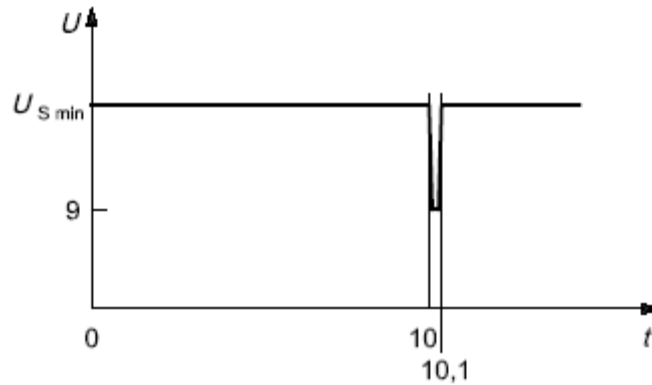


How to recall this waveform from menu (take 12V system as an example):

1. Click **Vehicle** on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **ISO16750-2** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Short-Drop** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Voltage Range** function setting and press the **[Enter]** key to confirm. Press the numeric keys to set the startup voltage as $V=12V$ and press **[Enter]** to confirm.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.

Reset-Test

This test verifies the reset behavior of the DUT at different voltage drops. This test is applicable to equipment with reset function, e.g. equipment containing microcontroller. Apply the test pulse simultaneously in figure below to all relevant inputs (connections) and check the reset behavior of the DUT. Decrease the supply voltage by 5 % from the minimum supply voltage, $U_{s \text{ min}}$, to $0.95 U_{s \text{ min}}$. Hold this voltage for 5 s. Raise the voltage to $U_{s \text{ min}}$. Hold $U_{s \text{ min}}$ for at least 10 s and perform a functional test. Then decrease the voltage to $0.95 U_{s \text{ min}}$. Continue with steps of 5 % of $U_{s \text{ min}}$, as shown in figure below, until the lower value has reached 0 V. Then raise the voltage to $U_{s \text{ min}}$ again.

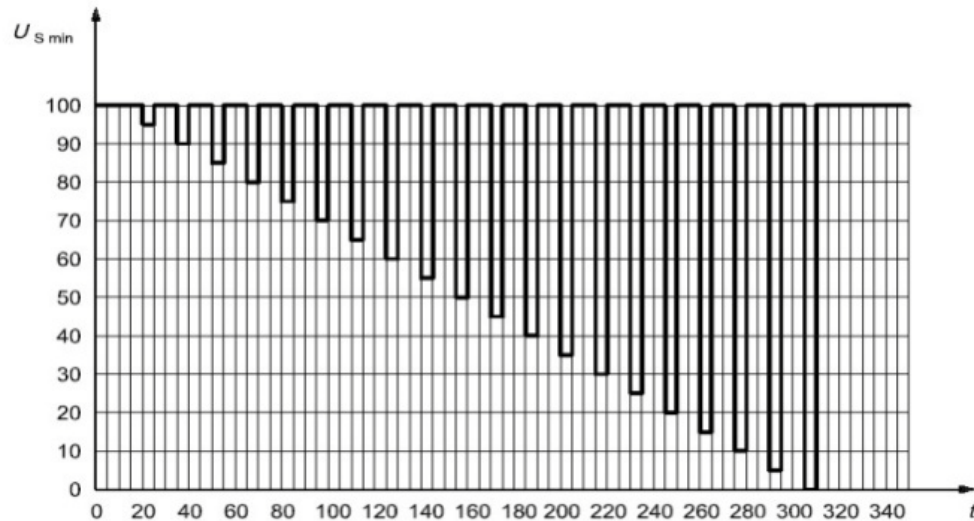


How to recall this waveform from menu is as below:

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **ISO16750-2** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Reset-Test** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Usmin** function setting and press the **[Enter]** key to confirm. Press the numeric keys to set the startup voltage as V=340V and press **[Enter]** to confirm.
2. Press **[On/Off]** on the front panel, turn on the output.
3. Press **[Run]** in the Vehicle function interface to output the voltage waveform.

Starting Waveform

Simulates the effects of rippled DC voltage on DC power when the car is started. From the constant voltage line in the original standard DIN40839 voltage waveform, the voltage curve in t8 duration is upgraded to a curve containing a 2Hz AC voltage waveform.

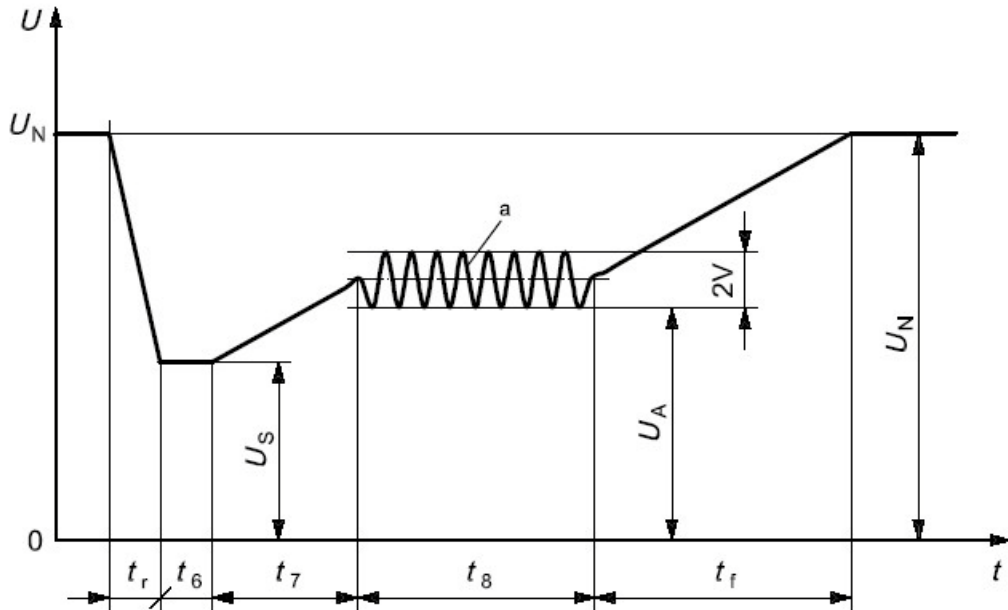

- Standards for 12V system:

Curve should be selected based on actual test requirements. To create waveform within 12V, follow the set standards as below:

| Levels/voltages/duration of starting profile | | | | |
|--|------------------------|------------------------|------------------------|------------|
| I | II | III | IV | Tolerances |
| $U_S = 8 \text{ V}$ | $U_S = 4,5 \text{ V}$ | $U_S = 3 \text{ V}$ | $U_S = 6 \text{ V}$ | + 0,2 V |
| $U_A = 9,5 \text{ V}$ | $U_A = 6,5 \text{ V}$ | $U_A = 5 \text{ V}$ | $U_A = 6,5 \text{ V}$ | |
| $t_r = 5 \text{ ms}$ | | | | ± 10 % |
| $t_6 = 15 \text{ ms}$ | | | | |
| $t_7 = 50 \text{ ms}$ | | | | |
| $t_8 = 1 \text{ s}$ | $t_8 = 10 \text{ s}$ | $t_8 = 1 \text{ s}$ | $t_8 = 10 \text{ s}$ | ± 10 % |
| $t_f = 40 \text{ ms}$ | $t_f = 100 \text{ ms}$ | $t_f = 100 \text{ ms}$ | $t_f = 100 \text{ ms}$ | |

- Standards for 24V system:

| Levels/voltages/duration of starting profile | | | |
|--|------------------------|-----------------------|------------|
| I | II | III | Tolerances |
| $U_S = 10 \text{ V}$ | $U_S = 8 \text{ V}$ | $U_S = 6 \text{ V}$ | + 0,2 V |
| $U_A = 20 \text{ V}$ | $U_A = 15 \text{ V}$ | $U_A = 10 \text{ V}$ | |
| $t_r = 10 \text{ ms}$ | | | ± 10 % |
| $t_6 = 50 \text{ ms}$ | | | |
| $t_7 = 50 \text{ ms}$ | | | |
| $t_8 = 1 \text{ s}$ | $t_8 = 10 \text{ s}$ | $t_8 = 1 \text{ s}$ | ± 10 % |
| $t_f = 40 \text{ ms}$ | $t_f = 100 \text{ ms}$ | $t_f = 40 \text{ ms}$ | |

How to recall this waveform from menu (take 12V system as an example):

1. Click **Vehicle** on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **ISO16750-2** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Starting-Profile** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Voltage Range** function setting and press the **[Enter]** key to confirm. Press the numeric keys to set the voltage as V=12V and press **[Enter]** to confirm.
 - 4) Press the up/down key to move the cursor to the **Profile Type** function setting and press the **[Enter]** key to confirm. Rotate the knob to select level **III** and press the **[Enter]** key to confirm.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.


Load Dump Dynamic Behavior

This test is a simulation of load dump transient occurring in the event of a discharged battery being disconnected while the alternator is generating charging current with other loads remaining on the alternator circuit at this moment.

- The amplitude of load dump is determined by the rotational speed of alternator and the strength of magnetic field in the case of disconnection of the battery.
- The pulse duration of load dump is mainly determined by the time constant and pulse amplitude of the excitation circuit.

Inside most novel alternator, the amplitude of load dump is decreased by increasing the limiter diode (clamping diode). The load dump may be caused by cable corrosion, poor cable contact or disconnecting the battery intentionally when the engine is running.

The pulse shape and parameters for an alternator without centralized load dump suppression (Test A) are given in follow.

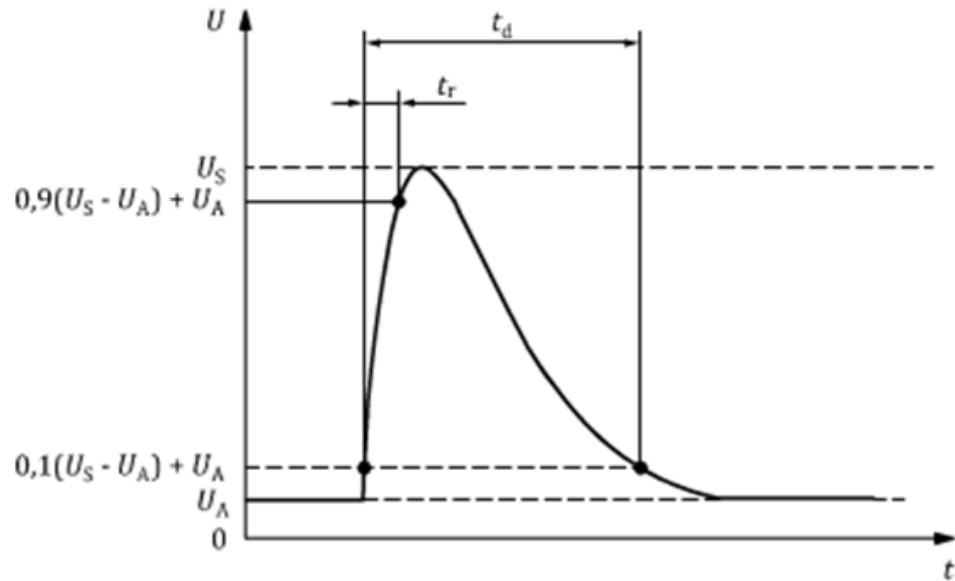


| Parameter | Type of system | | Minimum test requirements |
|----------------------|------------------------|-------------------------|-------------------------------|
| | 12V | 24V | |
| U_s^a (V) | $79 \leq U_s \leq 101$ | $151 \leq U_s \leq 202$ | 10 pulses at 1 min intervals. |
| R_i^a (Ω) | $0.5 \leq R_i \leq 4$ | $1 \leq R_i \leq 8$ | |
| t_d (ms) | $40 \leq t_d \leq 400$ | $100 \leq t_d \leq 350$ | |
| t_r (ms) | - | - | |

Note: ^a If not otherwise agreed, use the upper voltage level with the upper value for internal resistance or use the lower voltage level with the lower value for internal resistance.

- t: Time
- U: Test voltage.
- t_d : Duration of pulse.
- t_r : Rising Slope.
- U_A : The supply voltage of the generator in operation: $U_A = 14V$ in the 12V system, $U_A = 28V$ in the 24V system. (see ISO 16750-1).
- U_s : Peak voltage.

The pulse shape and parameters for an alternator with centralized load dump suppression (Test B) are given in follow.

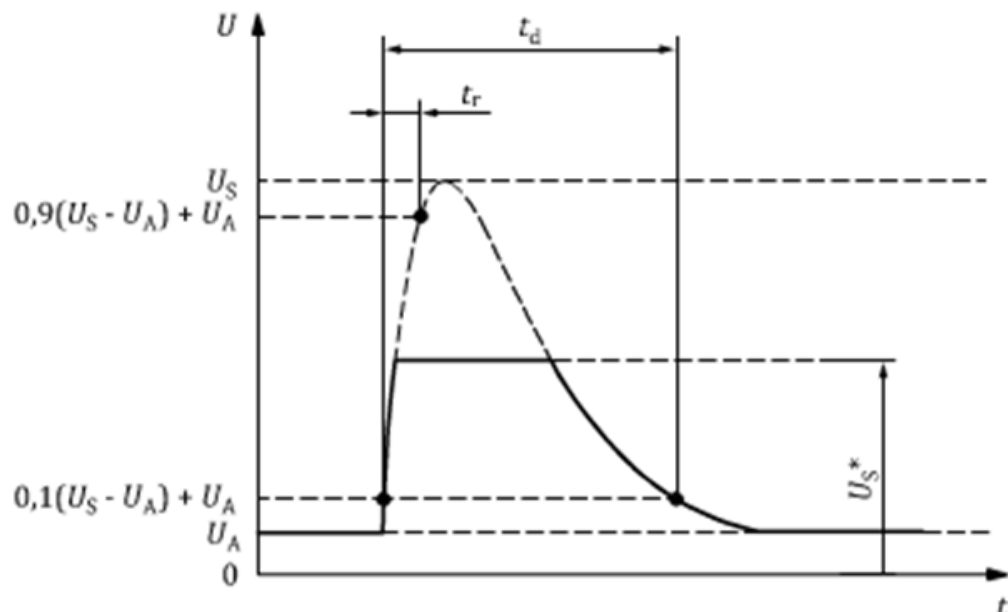

| Parameter | Type of system | | Minimum test requirements |
|---|--|--|---------------------------------|
| | 12V | 24V | |
| Us ^a (V) | 79≤Us≤101 | 151≤Us≤202 | 5 pulses at 1 minute intervals. |
| Us*(V) | It is fixed at 35V here and cannot be set. | As specified by customer (typical value 58). | |
| Ri ^a (Ω) | 0.5≤Ri≤4 | 1≤Ri≤8 | |
| t _d (ms) | 40≤t _d ≤400 | 100≤t _d ≤350 | |
| t _r (ms) | - | - | |
| Note: ^a If not otherwise agreed, use the upper voltage level with the upper value for internal resistance or use the lower voltage level with the lower value for internal resistance. | | | |
| <ul style="list-style-type: none"> ● t: Time ● U: Test voltage ● t_d: Duration of pulse ● t_r: Rising Slope ● U_A: The supply voltage of the generator in operation: U_A=14V in the 12V system, U_A=28V in the 24V system. (see ISO 16750-1) ● U_S: Peak voltage ● U_S*: Supply voltage with load dump suppression (i.e. clamping voltage) | | | |

The following general considerations of the dynamic behavior of alternators during load dump apply:

- The internal resistance of an alternator, in the case of load dump, is mainly a function of alternator rotational speed and excitation current.
- The internal resistance, Ri, of the load dump test pulse generator shall be obtained from the following relationship.

$$R_i = \frac{10 \times U_{\text{nom}} \times N_{\text{act}}}{0.8 \times I_{\text{rated}} \times 12000 \text{min}^{-1}}$$

- U_{nom}: The specified voltage of the alternator.
- I_{rated}: The specified current at an alternator speed of 6000r/min.
- N_{act}: The actual alternator speed, unit: round per minute (r/min).
- The pulse is determined by the peak voltage U_n, the clamping voltage U_S, the internal resistance Ri, and the pulse duration t_d; in all cases small values of U_n are correlated with small values of Ri and t_d, and high values of U_n with high values of Ri and t_d. For the test voltage U_A please refer to ISO16750-1.

How to recall this waveform from menu (take Test A 12V as an example):

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **ISO16750-2** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Load-Dump** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Voltage Range** function setting and press the **[Enter]** key to confirm. Press the numeric

- keys to set the voltage as $V=12V$ and press **[Enter]** to confirm.
- 4) Press the up/down key to move the cursor to the **Td** function setting and press the **[Enter]** key to confirm. Rotate the knob to set the duration of pulse and press the **[Enter]** key to confirm.
 - 5) Press the up/down key to move the cursor to the **U_n** function setting and press the **[Enter]** key to confirm. Rotate the knob to set the peak voltage and press the **[Enter]** key to confirm.
2. Press **[Run]** in the Vehicle function interface.
 3. Press **[On/Off]** on the front panel, turn on the output.
 4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.


4.7.3 ISO21848

A test wave completely conforming to International Standard ISO21848 is built inside the device, which can be used for the test of Electrical and electronic equipment for a supply voltage of 42V - Electrical loads. The user can directly and quickly recall this function during test.

U_{max,dyn} test pulse

Detect the function when the DUT is under maximum dynamic Voltage $U_{max,dyn}$, and simulate the maximum dynamic Voltage of high-energy pulse raised from throw load in 42V electrical system, where the upper limit is the protection voltage of throw load.

Apply 1 test pulse to the DUT, as shown below:

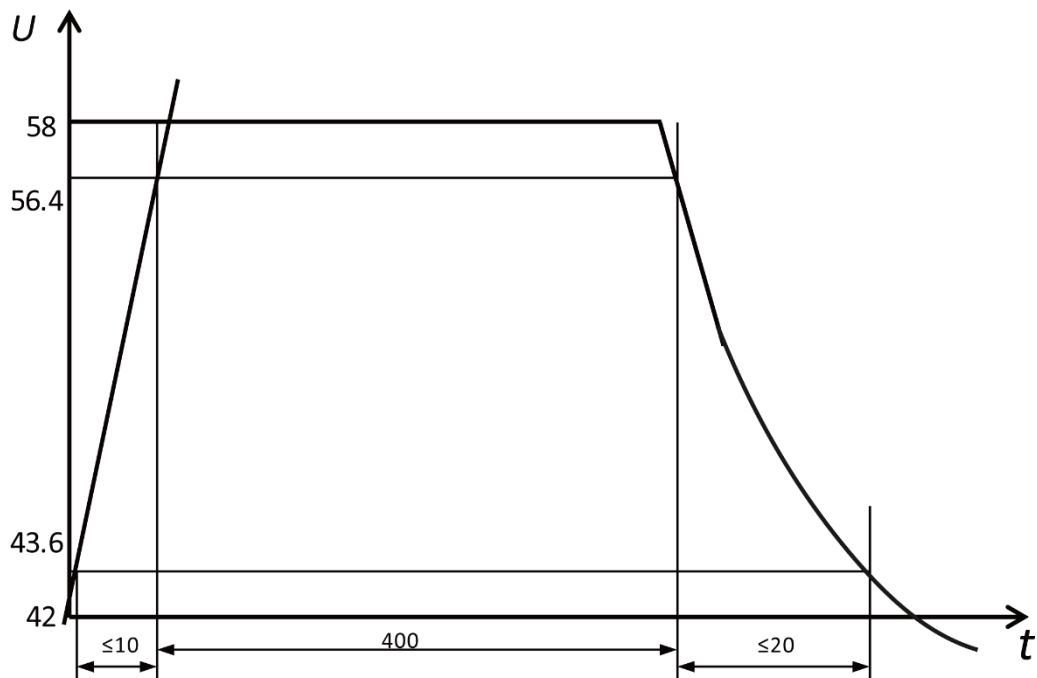


- t: time (in ms)
- U: Voltage (in V)

Supply Voltage Transient Drop (Drop_down)

Simulate the affect from short circuit when fuse element of another circuit is melt. Detect the function status of the DUT at transient drop of Voltage.

When the given test pulse is applied at all input terminals of the DUT, the rise and fall time between U_{low} and 16V level shall not be longer than 10ms.

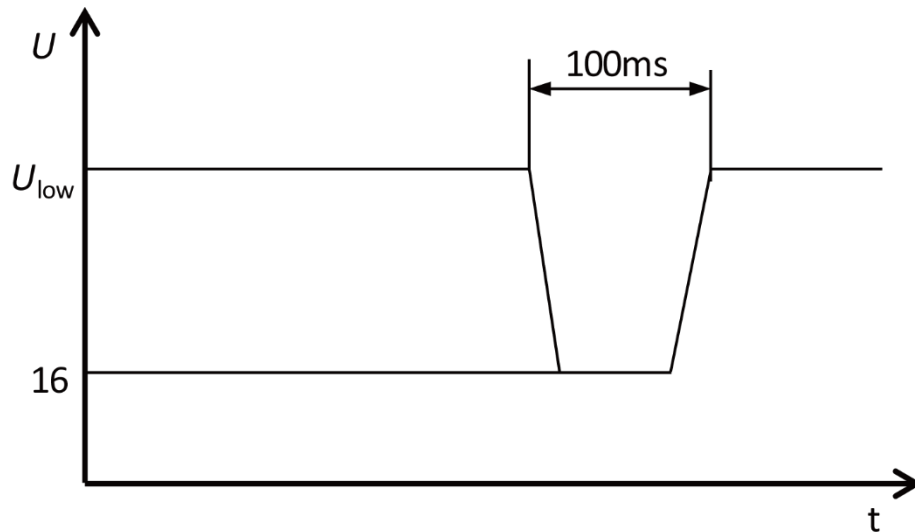


- t : time (in s)
- U : voltage (in V)

Reset Performance at Transient Drop of Voltage (Reset)

Detect the reset performance of the DUT at different Voltage drops. Applicable for devices with reset function (for example, device installed with one or several micro controllers).

As shown in the figure, apply test pulse and detect the reset performance of the DUT.

The supply voltage drops from U_{low} to $0.95U_{low}$ by 5% and keeps for 5s, and then rise to U_{low} and keep for at least 10s for function test. Then, drop Voltage to $0.9U_{low}$, and so on. As shown in the figure, drop the voltage from U_{low} to 0V by 5% and raise the voltage to U_{low} . The Rise and Fall time shall be between 10ms and 1s.

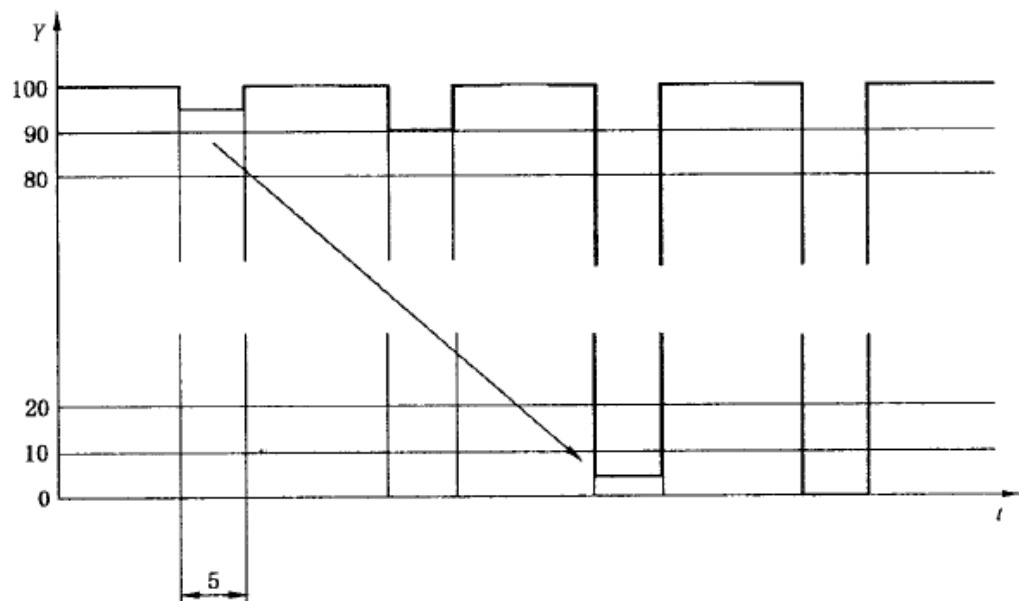


- t : time (in s)

- Y: Ulow, %

Start-up Characteristics (Start)

Detect DUT characteristics before and after vehicle startup.

Apply the startup characteristic parameters as shown in the figure and table to related input terminals of the DUT simultaneously.

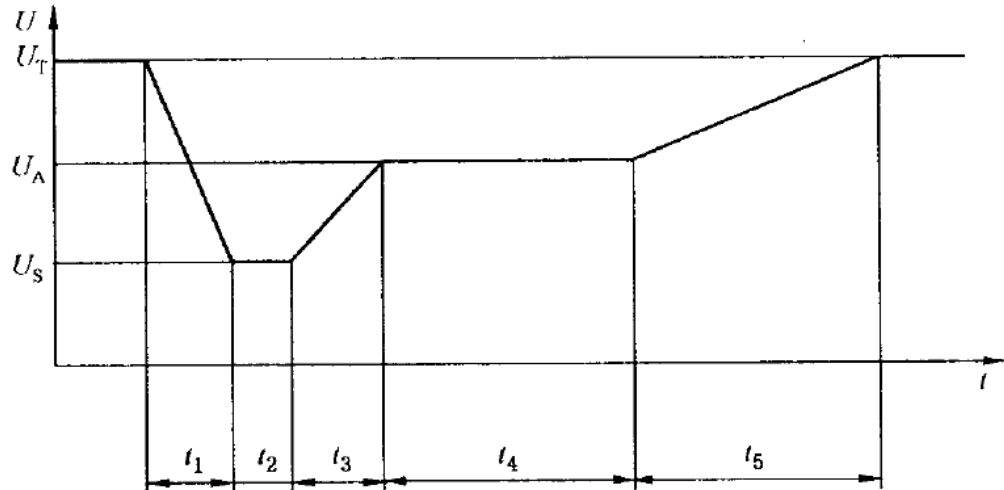

- t: time (in s) t1: 5ms
- U: voltage (in V) t2: 15ms
- U_S : 18V t3: 50ms
- U_A : 21V t4: 10000ms
- U_T : 42V t5: 100ms

How to Use


Take **Momentary-Drop** as an example to introduce the procedures as follows:

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **ISO21848** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Momentary-Drop** and press the **[Enter]** key to confirm.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.

4.7.4 SAEJ1113-11

Test - 2B


Transient from DC motors acting as generators after ignition switch OFF:

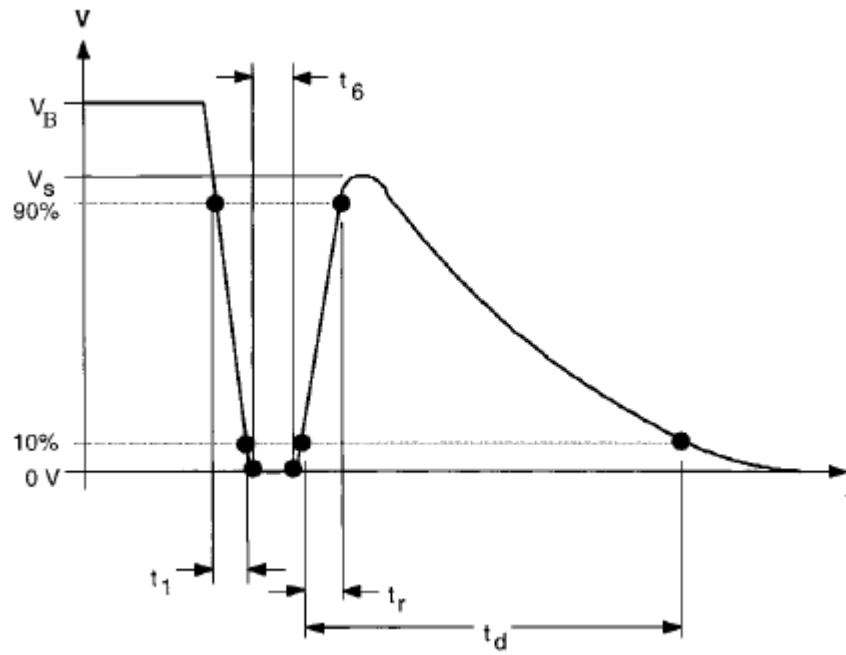

| Parameters | 12V | 24V |
|------------|-----------------------|-----------------------|
| V_s | 10V | 20V |
| R_i | $\leq 0.05\Omega$ | $\leq 0.05\Omega$ |
| t_d | 0.2 - 2s | 0.2 - 2s |
| t_1 | $1\text{ms} \pm 50\%$ | $1\text{ms} \pm 50\%$ |
| t_r | $1\text{ms} \pm 50\%$ | $1\text{ms} \pm 50\%$ |
| t_6 | $1\text{ms} \pm 50\%$ | $1\text{ms} \pm 50\%$ |

Test - 4

Starter motor engagement disturbance pulse.

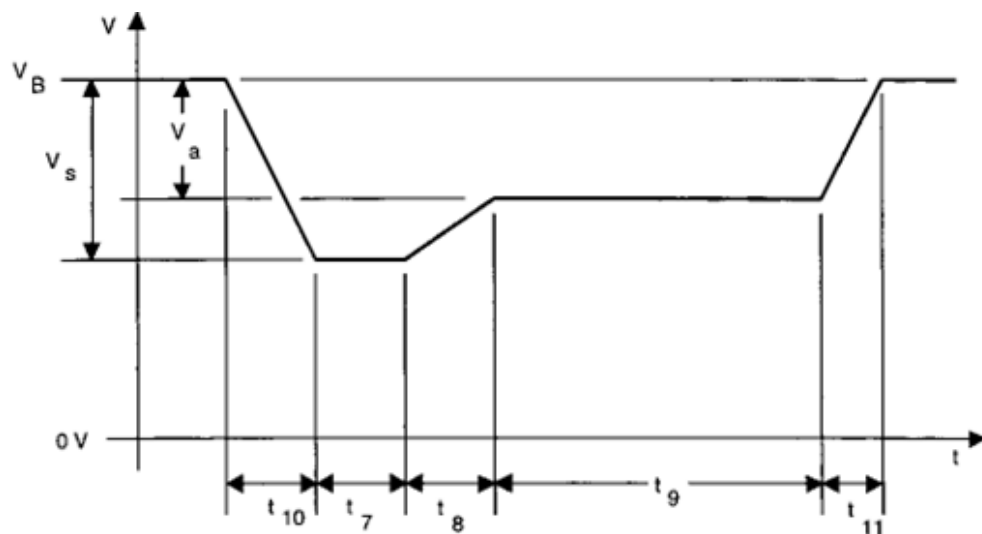

| Parameters | 12V | 24V |
|------------|-----|-----|
|------------|-----|-----|

| | | |
|---------------------|-------------------------------------|------------------------------------|
| V_s (From V_B) | -4V to -7V | -5V to -16V |
| V_a (From V_B) | -2.5 to -6V with $ V_a \leq V_s $ | -5 to -12V with $ V_a \leq V_s $ |
| R_i | 0Ω to 0.02Ω | 0Ω to 0.02Ω |
| t_7 | 15 to 40ms ⁽¹⁾ | 50 to 100ms ⁽¹⁾ |
| t_8 | ≤ 50 ms | ≤ 50 ms |
| t_9 | 0.5 to 20s ⁽¹⁾ | 0.5 to 20s ⁽¹⁾ |
| t_{10} | 5ms | 10ms |
| t_{11} | 5 to 100ms ⁽²⁾ | 10 to 100 ms ⁽³⁾ |

(1). The value used should be agreed between the vehicle manufacturer and the equipment supplier to suit the proposed application.

(2). $t_{11}=5$ ms is typical of the case when engine starts at the end of the cranking period, while $t_{11}=100$ ms is typical of the case when the engine does not start.

(3). $t_{11}=10$ ms is typical of the case when engine starts at the end of the cranking period, while $t_{11}=100$ ms is typical of the case when the engine does not start.

Test - 5

For the details, please refer to the [Load Dump Dynamic Behavior](#).

How to Use

Take Test - 2B as an example to introduce the procedures as follows:

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **SAEJ1113-11** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Test - 2B** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Voltage Range** function setting and press the **[Enter]** key to confirm. Press the numeric keys to set the voltage as $V=12V$ and press **[Enter]** to confirm.
 - 4) Press the up/down key to move the cursor to the **td** function setting and press the **[Enter]** key to confirm. Rotate the knob to set the duration of pulse and press the **[Enter]** key to confirm.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.

4.7.5 LV123

LV123 has been compiled for the electrical characteristics of new energy vehicles for major European car manufacturers. For its high-voltage system parts, the state standard within its operating voltage range is defined. The relevant parameters are introduced as follows:

WARNING


Please pay attention to whether the voltage value defined in the LV123 standard matches the rated voltage of the instrument, otherwise some waveforms cannot be recalled.

| LV123 waveform protocol | | | |
|-------------------------|--|---|---|
| Mode | Select the LV123 waveform editing method Curve or Userdefined. | | |
| | Curve | Choose to recall the standard LV123 waveform. | |
| | | Limit Range | |
| | | Unlimited | Range of unlimited operating capability, includes the following options: ● HV_1 ● HV_2a ● HV_2b ● HV_3 |
| | | Upperlimited | Range of upper limited operating capability, includes the following options: ● HV_1 ● HV_2a ● HV_2b ● HV_3 |
| | | Lowerlimited | Range of lower limited operating capability, includes the following options: ● HV_1 ● HV_2a ● HV_2b ● HV_3 |
| | | Highlylimited | Range of highly limited operating capability, includes the following options: ● HV_1 ● HV_2a ● HV_2b |
| | | Start voltage | Set the initial output voltage of the instrument before the LV123 regulation waveform test. At the same time, this value is also the end voltage after the regulatory waveform test is completed. |
| | | Start time | Test time of starting voltage, range: 0~999.999S. |
| | | End time | Test time of end voltage, range: 0~999.999S. |
| | | Count | Set the number of test repetitions, ranging from 1 to 65535. |
| | Userdefined | Select the user-defined LV123 waveform. | |
| | | Voltage Range | |
| | | Unlimited | Range of unlimited operating capability, |

| | | | | |
|--|--|---------------|---|---|
| | | | | with the following settings: V1: Voltage in interval 1 V2: Voltage in interval 2 V3: Voltage in interval 3 V4: Voltage in interval 4 |
| | | | Upperlimited | Range of upper limited operating capability, with the following settings: V1: Voltage in interval 1 V2: Voltage in interval 2 V3: Voltage in interval 3 V4: Voltage in interval 4 V5: Voltage in interval 5 V6: Voltage in interval 6 |
| | | | Lowerlimited | Range of lower limited operating capability, with the following settings: V1: Voltage in interval 1 V2: Voltage in interval 2 V3: Voltage in interval 3 V4: Voltage in interval 4 V5: Voltage in interval 5 V6: Voltage in interval 6 |
| | | | Highlylimited | Range of highly limited operating capability, with the following settings: V1: Voltage in interval 1 V2: Voltage in interval 2 V3: Voltage in interval 3 V4: Voltage in interval 4 V5: Voltage in interval 5 |
| | | Start voltage | Set the initial output voltage of the instrument before the LV123 regulation waveform test. At the same time, this value is also the end voltage after the regulatory waveform test is completed. | |
| | | Start time | Test time of starting voltage, range: 0~999.999S. | |
| | | End time | Test time of end voltage, range: 0~999.999S. | |
| | | Count | Set the number of test repetitions, ranging from 1 to 65535. | |

Unlimited

The waveform is as follows:

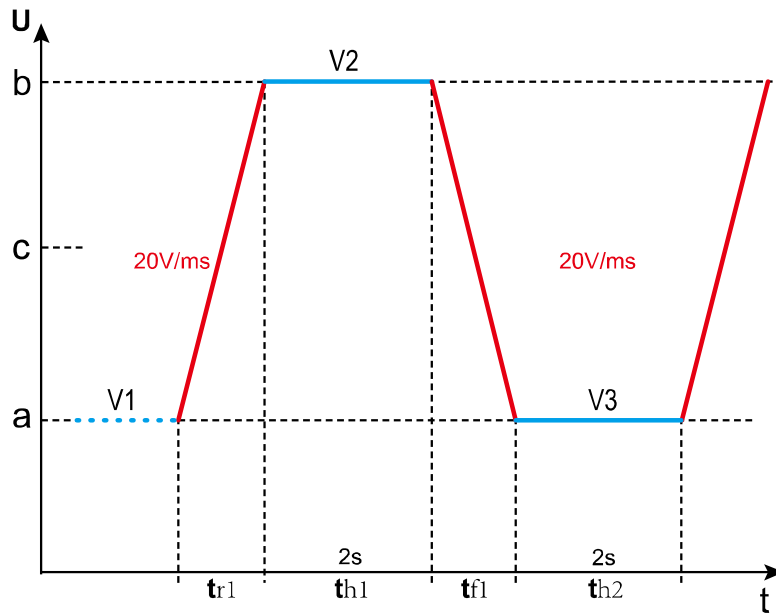


The parameters are as follows:

| Parameter | HV_1 | HV_2a | HV_2b | HV_3 |
|-----------|------|-------|-------|------|
| V1 | 90V | 170V | 250V | 520V |
| V2 | 190V | 340V | 450V | 750V |
| V3 | 90V | 170V | 250V | 520V |

Upper-limited

The waveform is as follows:

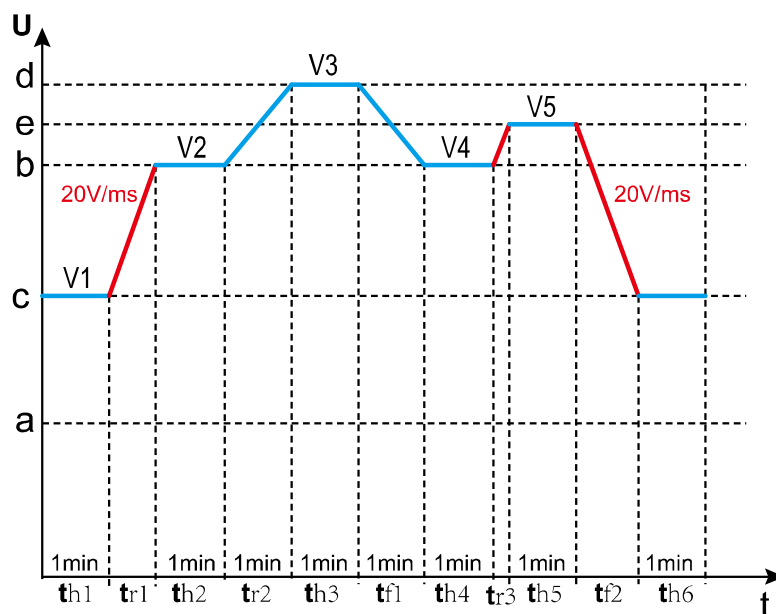


The parameters are as follows:

| Parameter | HV_1 | HV_2a | HV_2b | HV_3 |
|-----------|------|-------|-------|------|
| V1 | 140V | 255V | 350V | 635V |
| V2 | 190V | 340V | 450V | 750V |

| | | | | |
|----|------|------|------|------|
| V3 | 200V | 360V | 470V | 770V |
| V4 | 190V | 340V | 450V | 750V |
| V5 | 195V | 350V | 460V | 760V |

Lower-limited

The waveform is as follows:

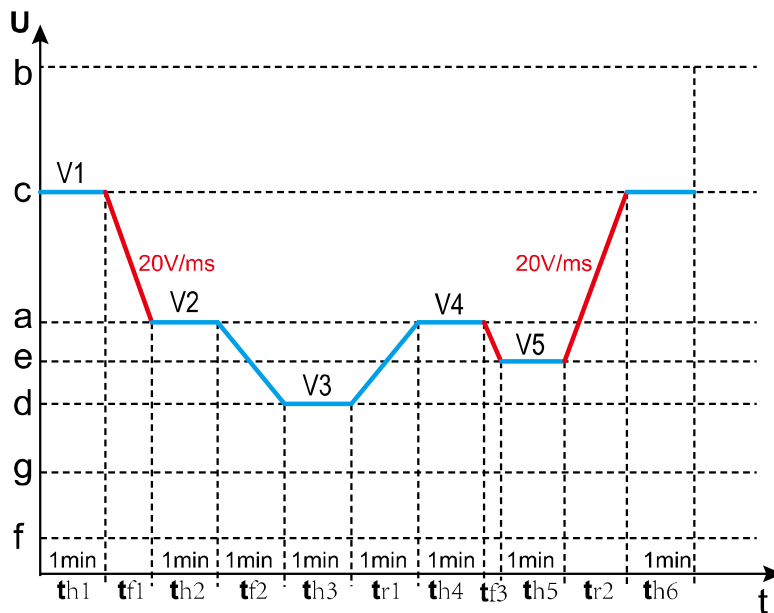


The parameters are as follows:

| Parameter | HV_1 | HV_2a | HV_2b | HV_3 |
|-----------|------|-------|-------|------|
| V1 | 140V | 255V | 350V | 635V |
| V2 | 90V | 170V | 250V | 520V |
| V3 | 80V | 160V | 200V | 450V |
| V4 | 90V | 170V | 250V | 520V |
| V5 | 85V | 165V | 225V | 485V |

Highly-limited

The waveform is as follows:

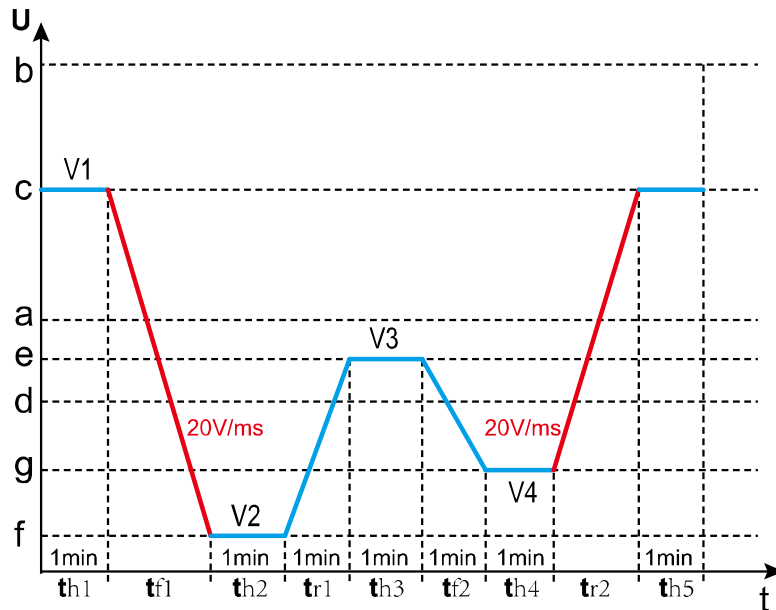

The parameters are as follows:

| Parameter | HV_1 | HV_2a | HV_2b | HV_3 |
|-----------|------|-------|-------|------|
| V1 | 140V | 255V | 350V | 635V |
| V2 | 60V | 120V | 150V | - |
| V3 | 85V | 165V | 225V | 485V |
| V4 | 70V | 140V | 175V | - |
| V5 | 140V | 255V | 350V | 635V |

How to Use

The following is an example of how to use this function by recalling the LV123 standard regulation Unlimited and HV_1 waveform.

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **LV123** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Curve** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Limit Range** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **unlimited** and press the **[Enter]** key to confirm.
 - 4) Press the up/down key to move the cursor to the **HV Range** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **HV_1** and press the **[Enter]** key to confirm.
 - 5) Set start voltage = 50V, start time = 0.1S, end time = 0.1S and count = 1.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press


[Shift]+[5](Trigger) to trigger the output of the waveform.

4.7.6 LV124

The built-in curves LV124 can meet general requirements, test conditions and tests of electrical and electronic components in motor vehicles up to 3.5 t.

E-01 Long-term overvoltage


The component's resistance to long-term overvoltage is tested. A generator control fault during driving operation is simulated.

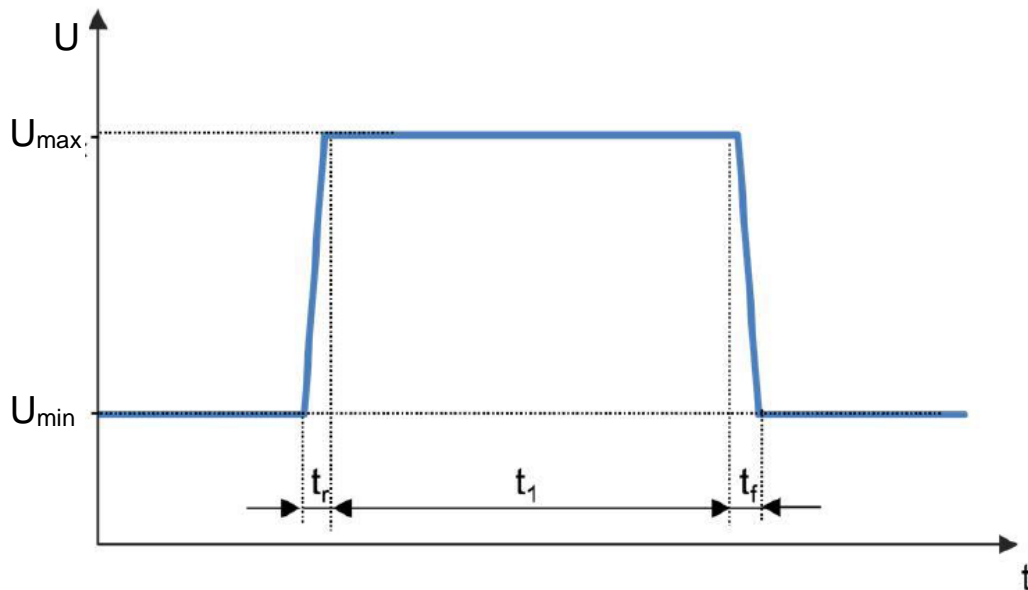

| Parameter | Description |
|-----------|-------------|
| U_{max} | 17V |
| U_{min} | 13.5V |
| t_r | <10ms |
| t_1 | 3600s |
| t_f | <10ms |

E-02 Transient Overvoltage Pulse


Transient overvoltages may occur in the electric system due to the switching off of loads and due to short accelerator tip-ins. These overvoltages are simulated by means of this test. This test may be used for the electrical life test. The test pulse of E-02 Transient overvoltage is shown in the figure below:

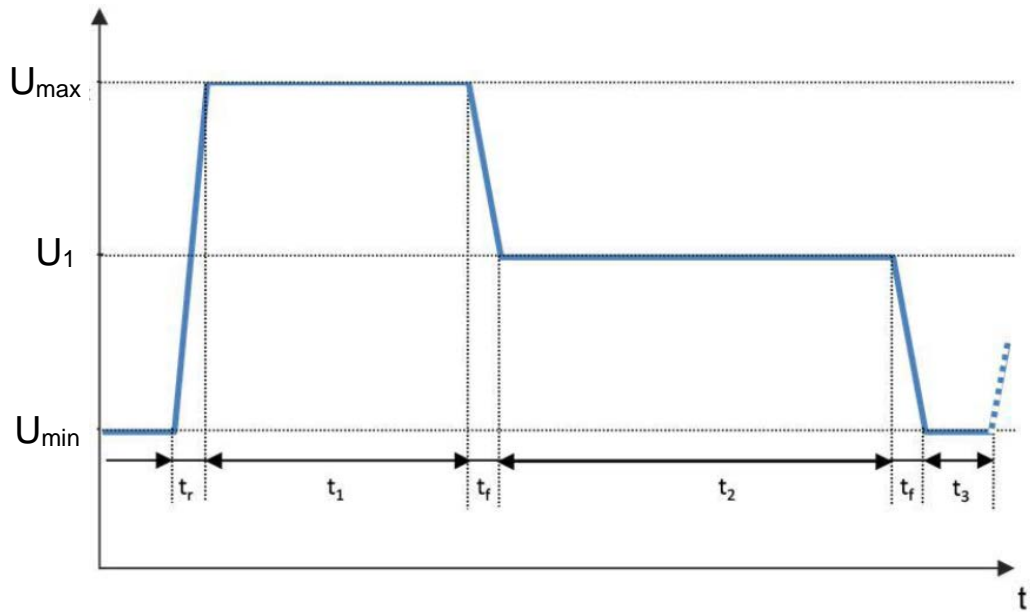

| Parameter | Description |
|-----------|-------------|
| U_{max} | 18V |
| U_1 | 17V |
| U_{min} | 13.5V |
| t_r | <10ms |
| t_1 | 400ms |
| t_f | <10ms |
| t_2 | 600ms |
| t_3 | 2s |
| Cycles | Short Test |

E-03 Transient undervoltage


Transient undervoltages in the electric system may occur due to switching on of loads. These undervoltages are simulated by means of this test.

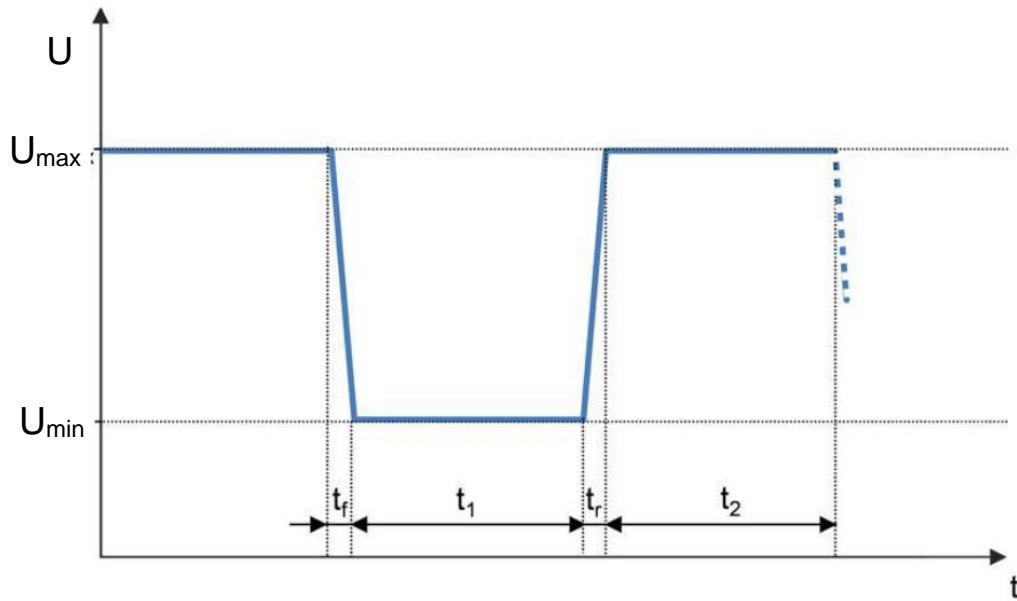

| Parameter | Description |
|------------|-------------|
| U_{\max} | 10.8V |
| U_{\min} | 9V |
| t_f | 1.8ms |
| t_1 | 500ms |
| t_r | <1.8ms |
| t_2 | 1s |
| Cycles | 1 |

E-04 Jump Start


External starting of the vehicle is simulated. The maximum test voltage results from commercial vehicle systems and their increased power supply voltage. The test pulse of E-04 Jump start is shown in the figure below:

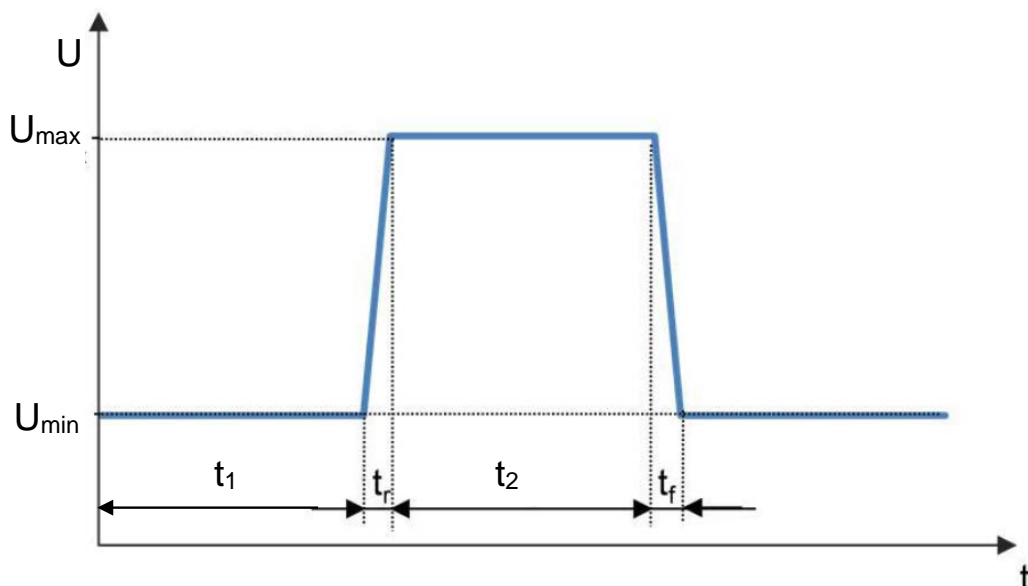

| Parameter | Description |
|-----------|-------------|
| U_{max} | 26V |
| U_{min} | 13.5V |
| t_1 | 60s |
| t_r | <10ms |
| t_2 | 60s |
| t_f | <10ms |

E-05 Load Dump


Dumping of an electric load, in combination with a battery with reduced buffering ability, results in an energy-rich overvoltage pulse due to the generator characteristics. The test pulse of E-05 Load Dump is shown in the figure below:

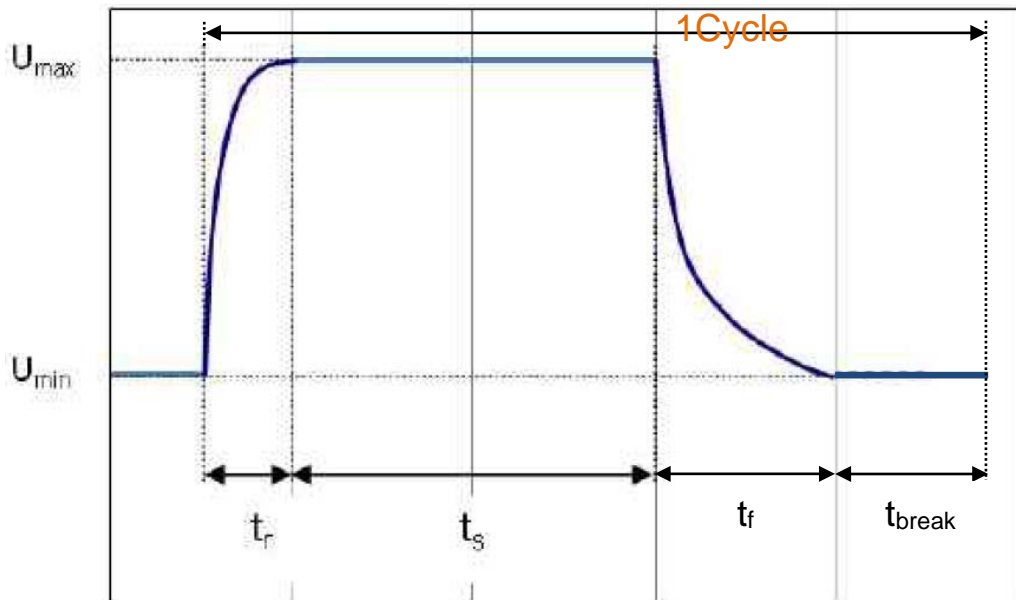

| Parameter | Description |
|-------------|-------------|
| U_{max} | 27V |
| U_{min} | 13.5V |
| t_r | <10ms |
| t_s | 300ms |
| t_f | <300ms |
| t_{break} | 60s |
| Cycles | 10 |

E-07 Slow Decrease and Slow Increase of the Supply Voltage


The slow decrease and increase of the supply voltage is simulated as it occurs during the slow discharging and charging procedure of the vehicle battery. The waveform is as follows.

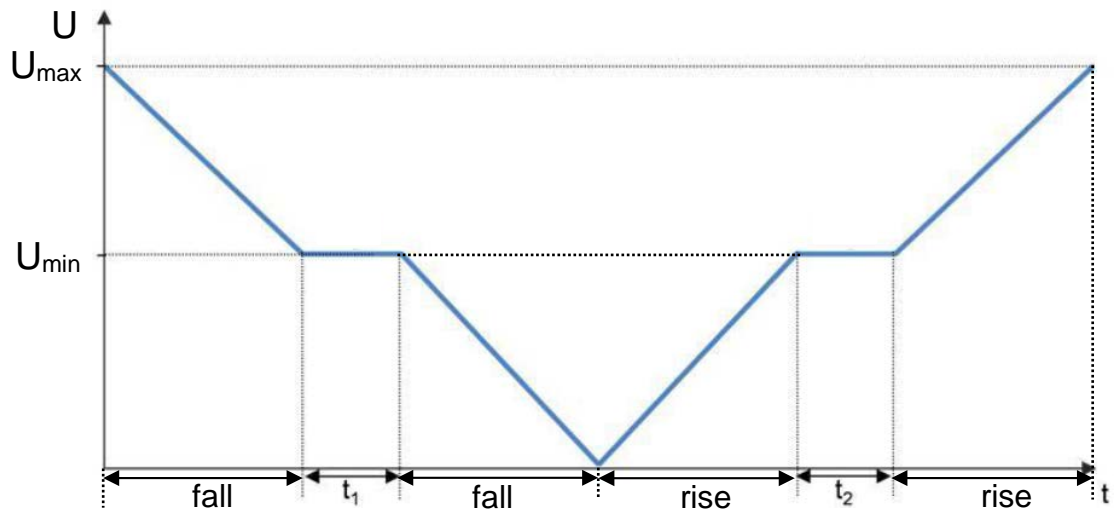

| Parameter | Description |
|-----------|-------------|
| U_{max} | 16V |
| U_{min} | 9V |
| t_1 | 60s |
| t_2 | 60s |
| rise | 0.5V/min |
| fall | 0.5V/min |

E-08 Slow Decrease and Quick Increase of the Supply Voltage

This test simulates the slow decrease of the battery voltage to 0 V and the sudden reconnection of the battery voltage e.g. by means of applying a jump start source. The waveform is as follows.

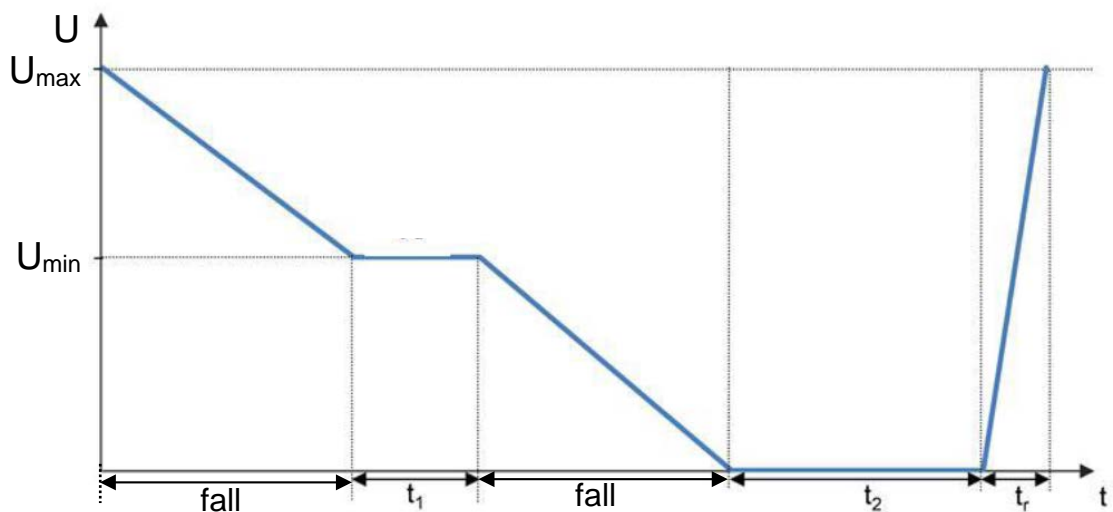


| Parameter | Description |
|-----------|-------------|
| U_{max} | 16V |
| U_{min} | 9V |

| | |
|----------------|----------|
| t1 | 60s |
| t2 | 60s |
| t _r | <0.5s |
| fall | 0.5V/min |

E-09 Reset Behavior

The reset behavior of a component in its environment is simulated and tested. Test boundary conditions (e.g. assembly, terminal, system) must be described in detail.

During operation, an arbitrary sequence of repeated switching-on/off procedures occurs; this must not lead to an undefined behavior of the component. The reset behavior is represented by a voltage variance and a time variance. Two different test sequences are required to simulate different switchoff times. A component must always undergo both sequences.

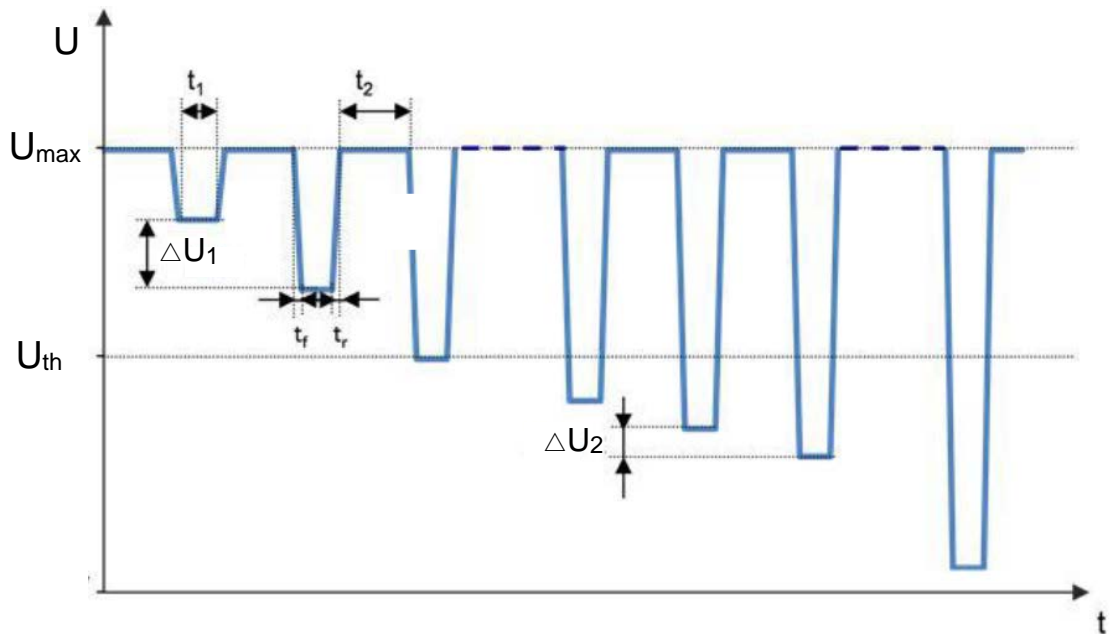


| Parameter | Description |
|------------------|-------------|
| U _{max} | 9.8V |
| U _{th} | 6V |
| ΔU ₁ | 0.5V |
| ΔU ₂ | 0.2V |
| t1 | 5s |
| t2 | >=10s |
| t _r | <=10ms |
| t _f | <=10ms |

E-11 Start Pulses


When starting the engine, the battery voltage drops to a low value for a short period and then slightly rises again. Most components are activated directly before starting for a short period, then deactivated during starting and activated again after starting when the engine is running. This test serves to verify normal operation under these conditions. The starting process may be performed under different vehicle starting conditions, cold start and warm start. In order to cover both cases, two different test sequences are required. A component must always undergo both sequences.

- Cold Start Test Pulse

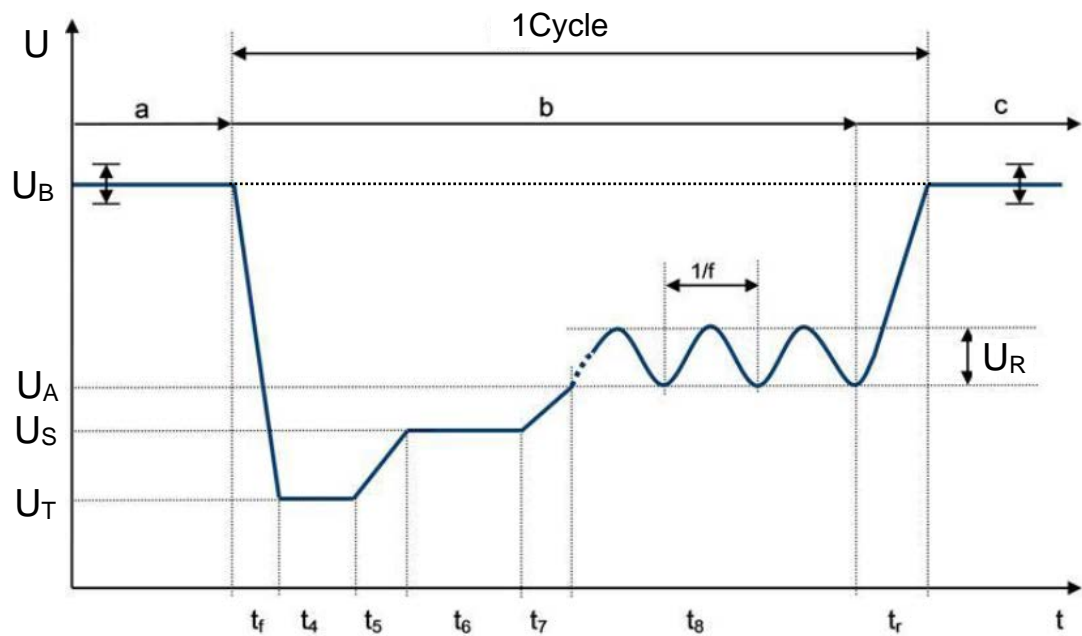

| Parameter | Description |
|-----------|-------------|
| U_B | 18V |
| U_A | 13.5V |
| U_S | 17V |
| U_T | |
| U_R | |
| t_f | 1ms |
| t_4 | 0ms |
| t_5 | 0ms |
| t_6 | 19ms |
| t_7 | 50ms |
| t_8 | 10ms |
| t_r | 100ms |
| freq | 2Hz |
| cycles | 10 |
| testseq | Short/Long |


- Warm Start Test Pulse

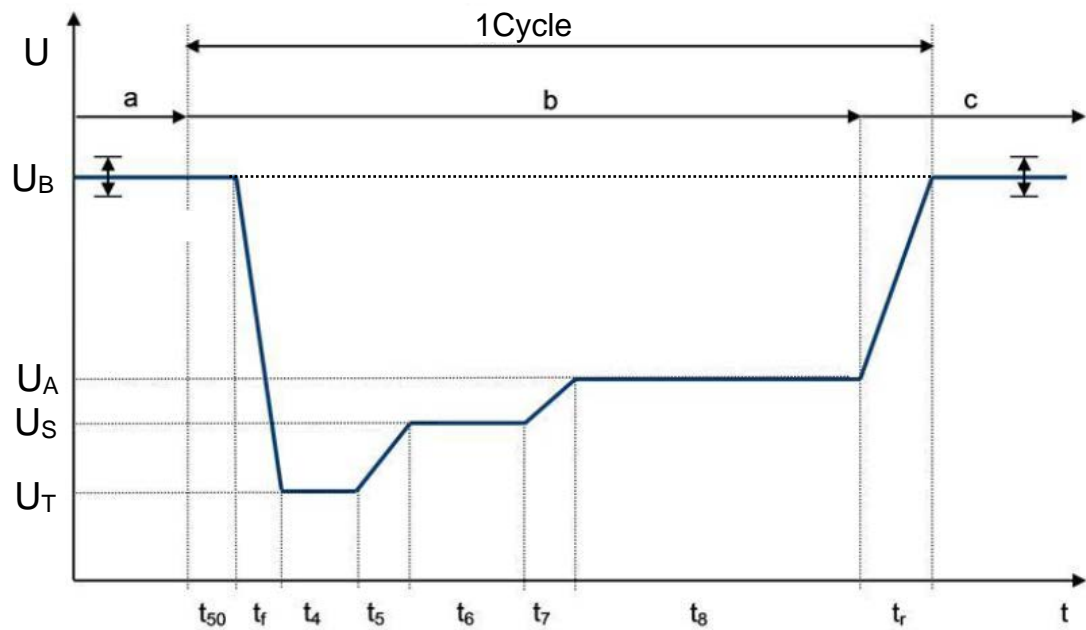

| Parameter | Description |
|-----------|-------------|
| U_B | 18V |
| U_A | 13.5V |
| U_S | 17V |
| U_T | |
| t_f | 1ms |
| t_4 | 0ms |
| t_5 | 0ms |
| t_6 | 19ms |
| t_7 | 50ms |
| t_8 | 10ms |
| t_r | 100ms |
| cycles | 10 |
| testseq | Short/Long |

E-12 Voltage Curve with Intelligent Generator Control

The behavior of the electric system when intelligent generator controls are used is simulated.

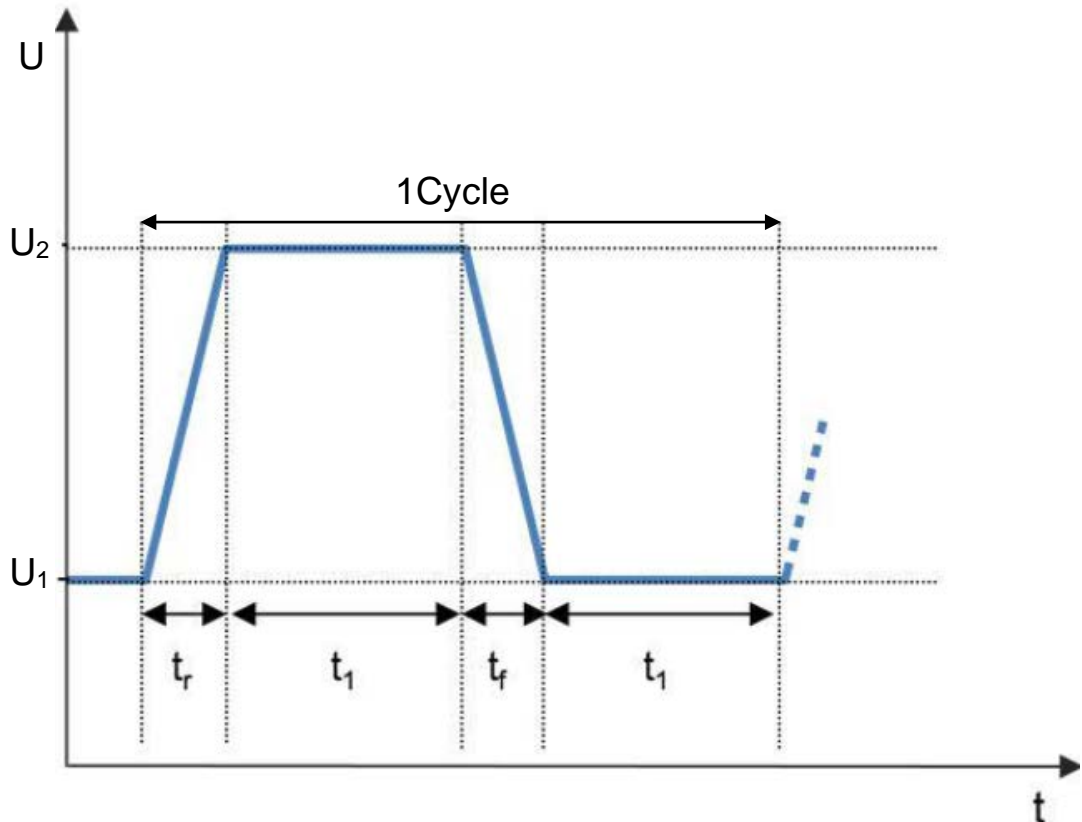

| Parameter | Description |
|-----------|---------------------|
| U_1 | 11.8V |
| U_2 | 15V |
| t_f | $\geq 300\text{ms}$ |
| t_r | |
| t_1 | 2s |
| cycles | 10 |

How to Use


The following is an example of how to use this function by recalling the LV124 standard regulation E-01 test.

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **LV124** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Testings** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **E-01** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Testcase** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Standard** and press the **[Enter]** key to confirm.
 - 4) Set $U_{\max} = 17\text{V}$, $U_{\min} = 13.5\text{V}$, $t_r < 10\text{ms}$, $t_1 = 3600\text{s}$ and $t_f < 10\text{ms}$.
2. Press **[Run]** in the Vehicle function interface.

3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.


4.7.7 LV148

LV148 covers tests for electric and electronic components in motor vehicles 48V electrical system. The voltage level and definition are shown in the figure below.

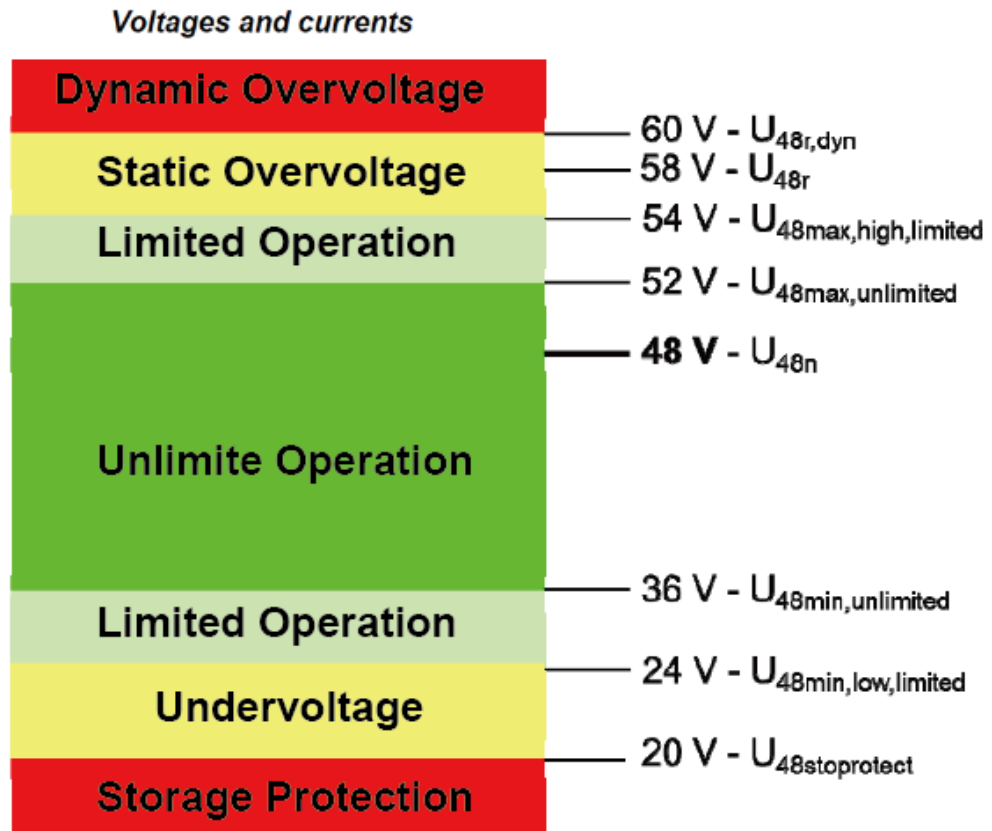

E-01a Long-term overvoltages


The component's resistance to long-term overvoltage is tested. A generator control fault during driving operation is simulated.

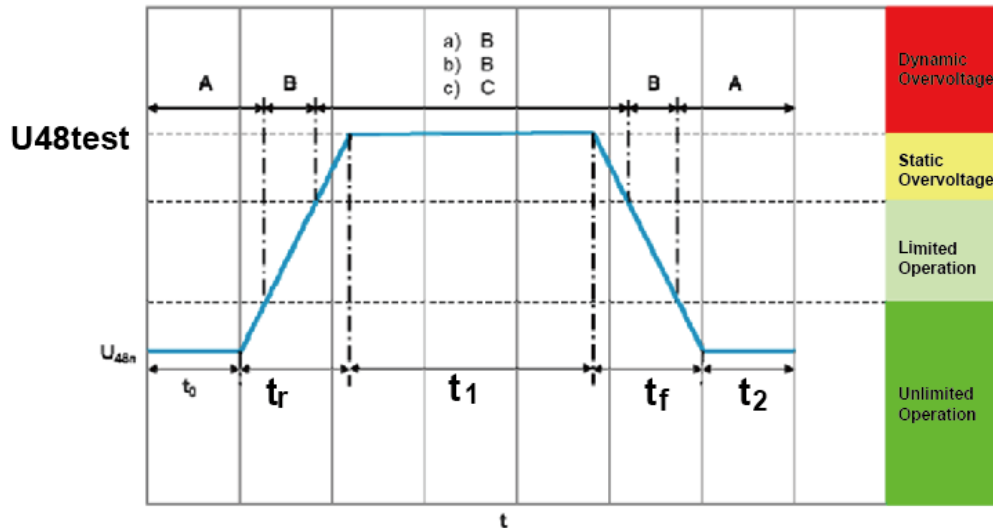

- t_r 0.1 s
- t_1 60 min.
- t_f 0.1 s
- t_2 1 s
- Test voltage U_{48test} $U_{48r,dyn}$

E-01b Long-term overvoltages on recuperating components


Testing for recuperation components in the electrical system where the energy can not be removed and therefore it results in a over voltage.

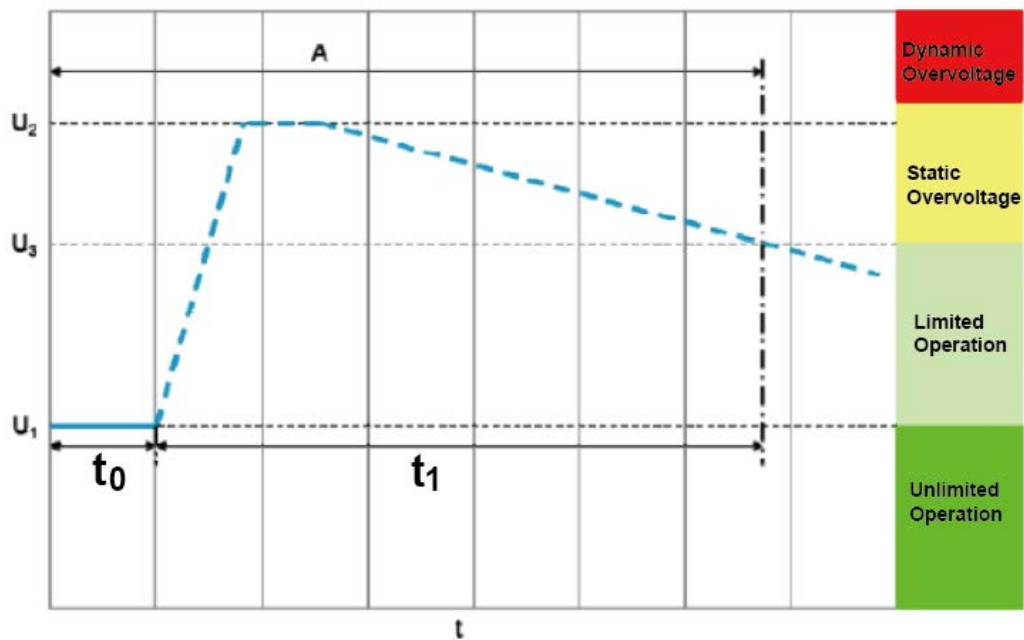

- t_0 $\geq 1s$
- t_1 $\leq 300ms$
- U_1 52V
- U_2 60V
- U_3 54V

E-02 Transient overvoltages


Transient overvoltages may occur in the electric system due to the switching off of loads and due to short accelerator tipins. These overvoltages are simulated by means of this test.

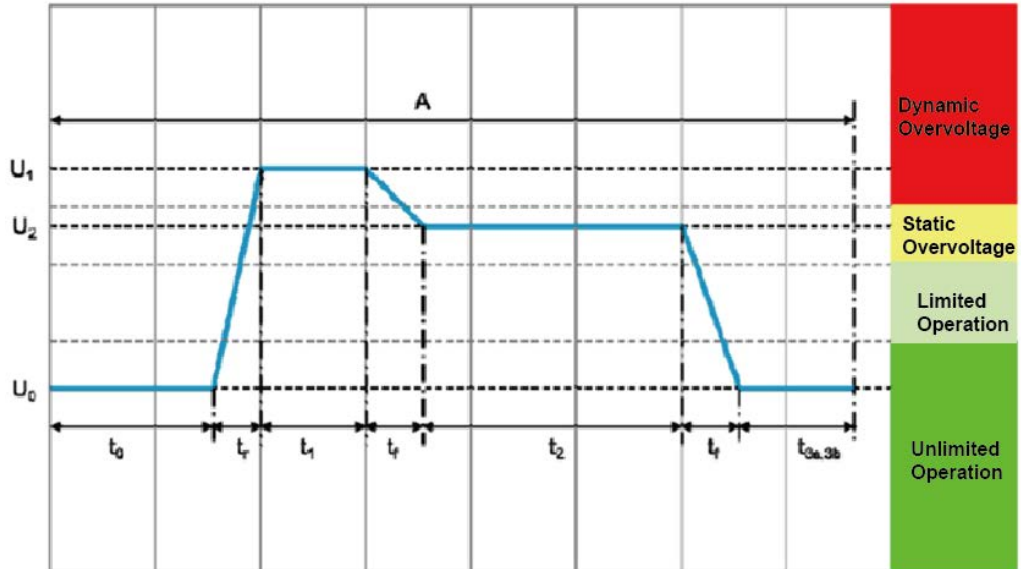

- | | |
|---------------------|---|
| • U_0 | U_{48n} |
| • U_1 | 70 V |
| • U_2 | U_{48r} |
| • t_0 | 100 ms |
| • t_r | 1 ms |
| • t_1 | 40 ms |
| • t_r | 1 ms |
| • t_2 | 600 ms |
| • t_{3a} | 2.5 s |
| • t_{3b} | 9 s |
| • R_i | $10 \text{ m}\Omega \leq R_i \leq 100 \text{ m}\Omega$ |
| • Number of cycles: | 1- Short test: 3 times with t_{3b} 2- Endurance test: 1000 times with t_{3b} |

E-03 Transient undervoltages

Transient undervoltages in the electric system may occur due to switching on of loads. These undervoltages are simulated by means of this test.

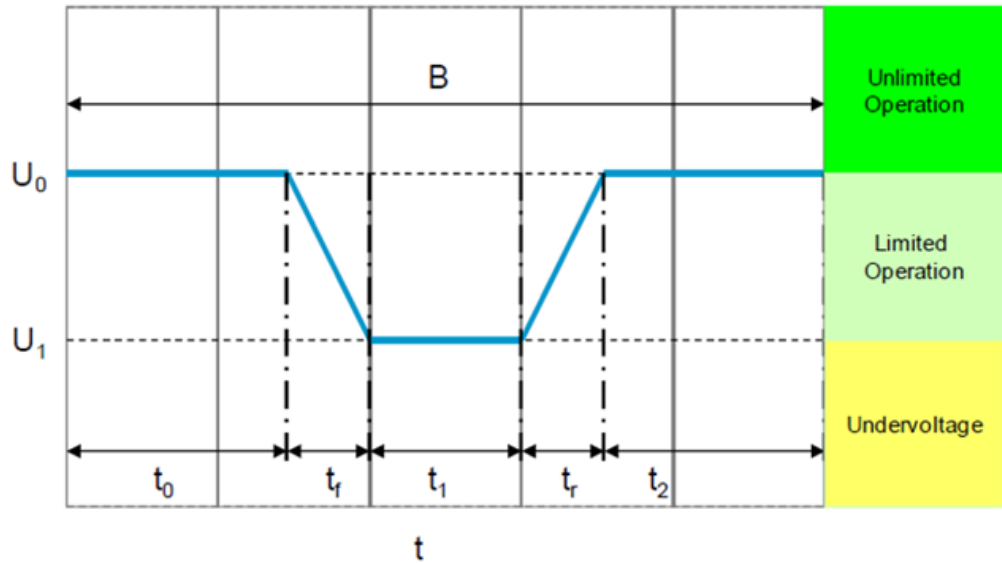


▸ Test parameters:

- | | |
|---------------------|--------------------------------|
| • U_0 | $U_{48\text{min,unlimited}}$ |
| • U_1 | $U_{48\text{min,low,limited}}$ |
| • t_0 | 60 s |
| • t_r | 2 ms |
| • t_1 | 500 ms |
| • t_r | 2 ms |
| • t_2 | 500 ms |
| • Number of cycles: | 1 |

E-04 Jumpstart / recuperation

Jump starting of the vehicle is simulated. The maximum test voltage results from commercial vehicle systems and their elevated electric system voltages.

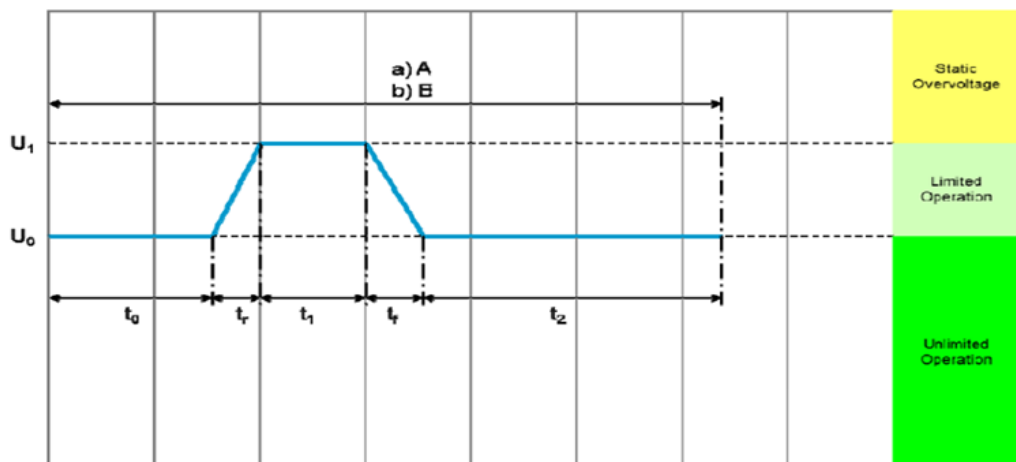


Test parameters:

| | |
|---------------------|--------------------------|
| • U_0 | $U_{48max,unlimited}$ |
| • U_1 | $U_{48max,high,limited}$ |
| • t_0 | 60 s |
| • t_r | 100 ms |
| • t_1 | 60 s |
| • t_f | 100 ms |
| • t_2 | 60 ms |
| • Number of cycles: | 1 |

E-06A Slow decrease and increase of the supply voltage (without energy storage)


The slow decrease and increase of the supply voltage is simulated as it occurs during the slow discharging and charging procedure of the vehicle battery.

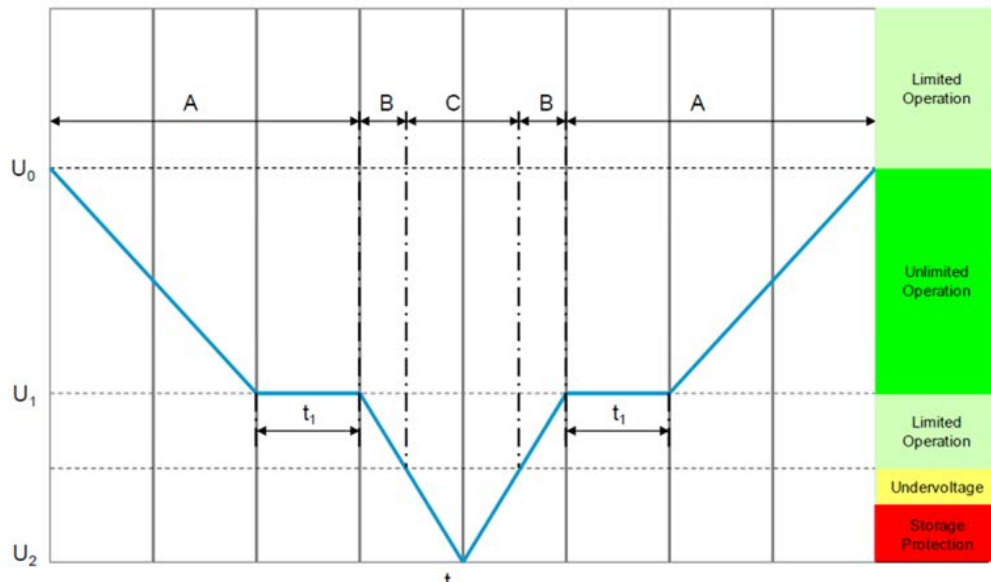
Test parameters:

| | |
|-----------------------------------|-----------------------|
| • U_0 | $U_{48max,unlimited}$ |
| • Voltage gradient (ΔU) | $\pm 2 \text{ V/min}$ |
| • U_1 | $U_{48min,unlimited}$ |
| • U_2 | 0 V |
| • t_1 | Holding Time |
| • Number of cycles: | 1 |

E-06B Slow decrease and increase of the supply voltage (with energy storage - Part 1)

Checks will slow the supply voltage decrease to the energy storage protection voltage, followed by energy storage disconnection.

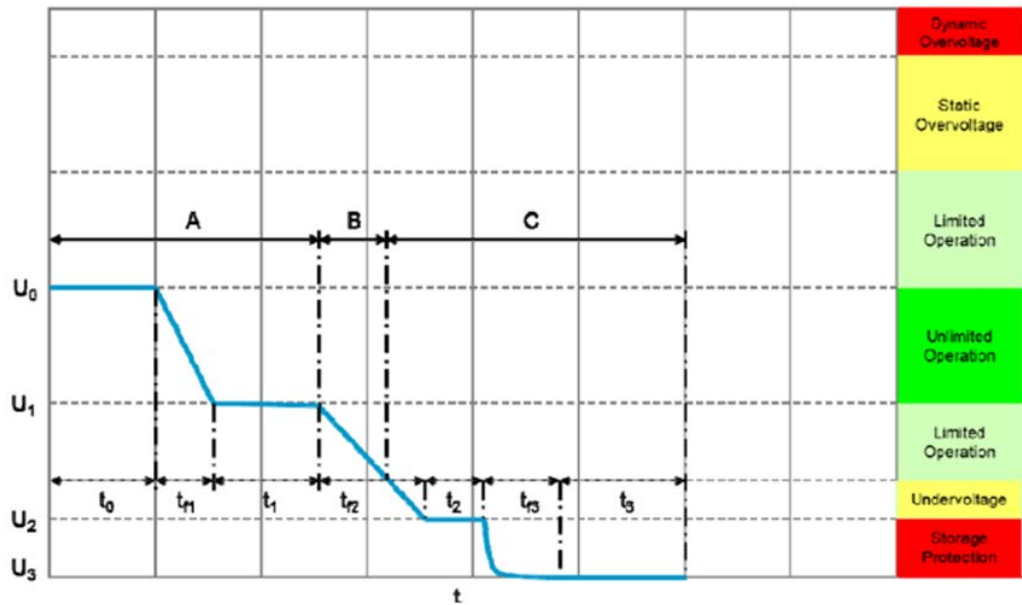


Test parameters:

- | | |
|---------------------|-------------------------|
| • U_0 | U_{48max} , unlimited |
| • U_1 | U_{48min} , unlimited |
| • U_2 | $U_{48stopprotect}$ |
| • U_3 | 0V |
| • t_0 | 100ms |
| • t_{f1} | 8min |
| • t_2 | 60s |
| • Number of cycles: | 1 |

E-07 Slow decrease, fast increase in the supply voltage

This test simulates the slow decrease of the vehicle system voltage to the energy storage protection voltage followed by shutdown to 0V and the sudden reconnect the system voltage by a charged or new energy storage battery.

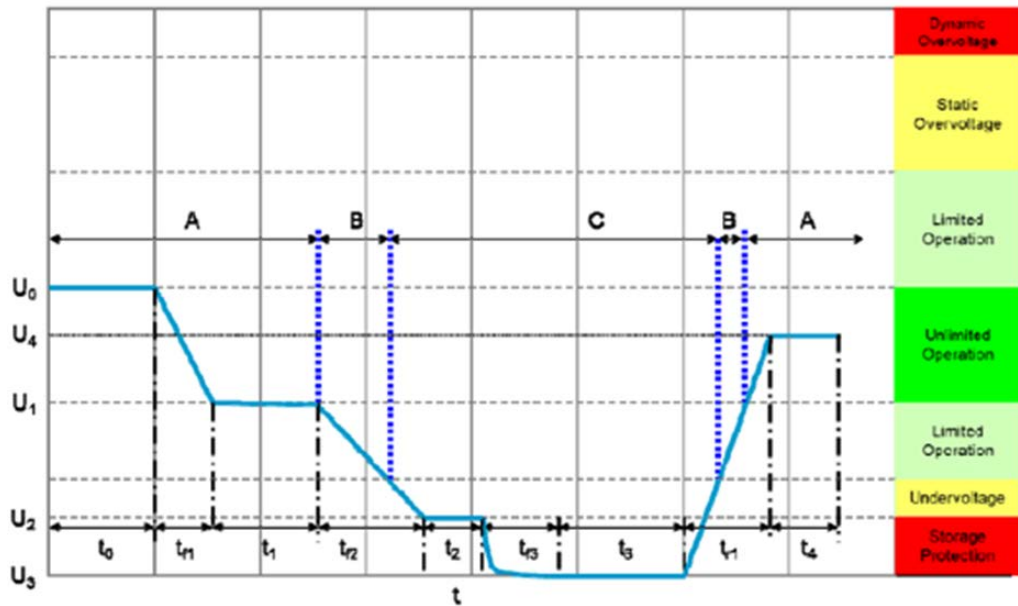


Test parameters:

- | | |
|---------------------|------------------------------|
| • U ₀ | U _{48max,unlimited} |
| • U ₁ | U _{48min,unlimited} |
| • U ₂ | U _{48stopprotect} |
| • U ₃ | 0 V |
| • U ₄ | U _{48n} |
| • t ₀ | 100ms |
| • t _{r1} | 8 min |
| • t ₁ | ≥60s |
| • t _{r2} | 8 min |
| • t ₂ | 60 s |
| • t _{r3} | 60 s |
| • t ₃ | 300 s |
| • t _{r1} | ≤ 100 ms |
| • t ₄ | 100 ms |
| • Number of cycles: | 1 |

E-08 Reset behavior


The reset behavior of a component in its environment is simulated and tested. Test boundary conditions (e.g., assembly, terminal, system) must be described in detail. During operation, an arbitrary sequence of repeated switching-on/off procedures occurs; this must not lead to an undefined behavior of the component. The reset behavior is represented by a voltage variance and a time variance. Two different test sequences are required to simulate different switch-off times. A component must always undergo both sequences.

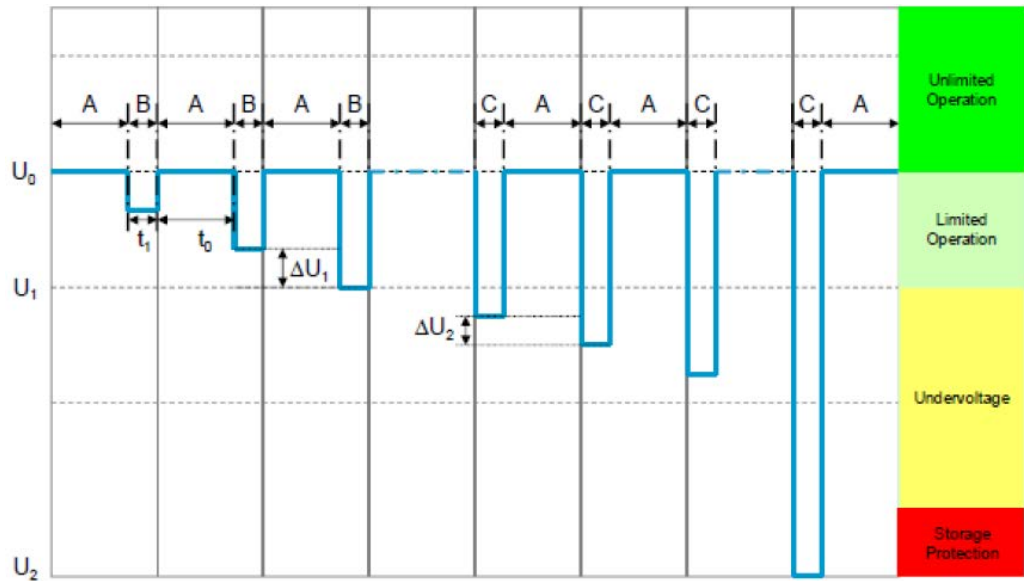

- t_0 $\geq 10s$
- t_1 $5s$
- t_r $\leq 100ms$
- t_f $\leq 100ms$
- U_0 $52V$
- U_1 $24V$
- U_2 $0V$
- ΔU_2 $0.5V$
- ΔU_1 $2V$

E-10 Start impulses

During a cold start (motor start), the energy storage battery voltage decreases for a short, then increases again. The warm start is not considered, because the operating range is maintained.

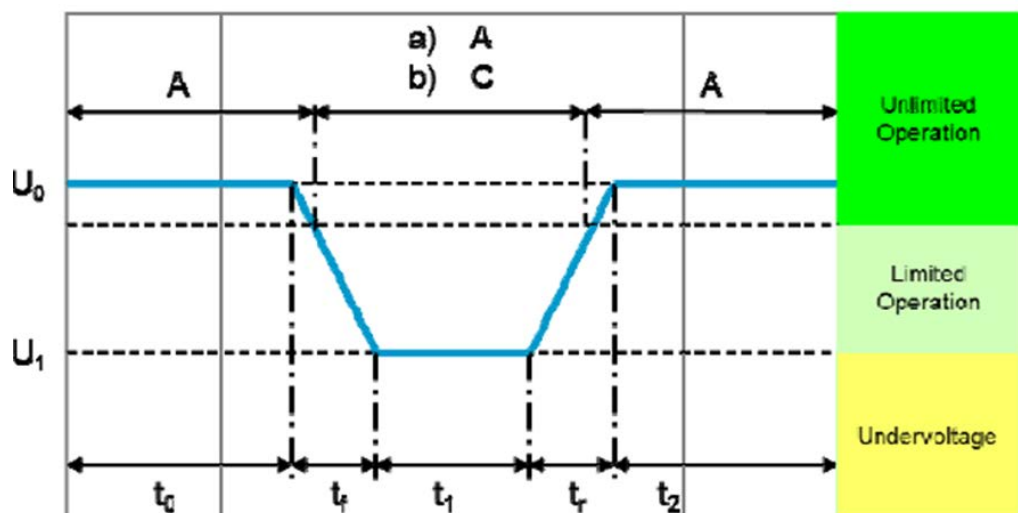


E-15 Test pulse parameters for E48-10 Starting pulses

| Parameters | Test pulse "normal" |
|-------------|---|
| Test pulse | Test pulse "normal" and "severe" |
| U_0 | U_{48n} for cold start normal 40 V for cold start severe |
| U_1 | $U_{48min,low,limited}$ |
| t_0 | 2s |
| t_f | 1ms |
| t_1 | 1s |
| t_r | 1 ms |
| t_2 | 2s |
| Test cycles | 10 |

E-15

Operation in the range without function restriction. The operating behavior at the range limits is checked.

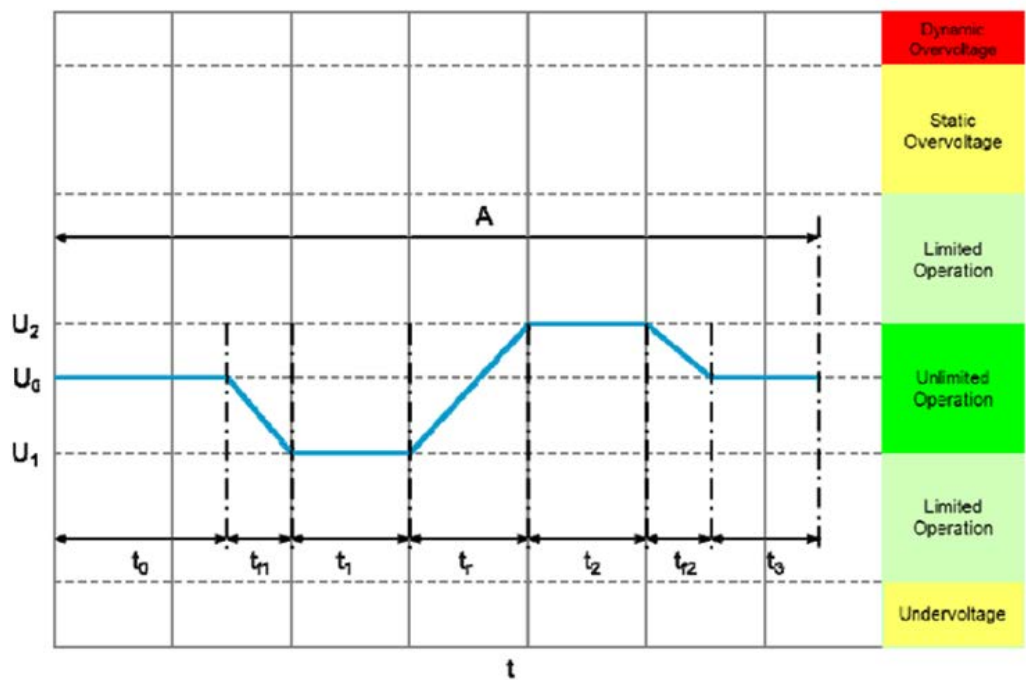


Test parameters:

| | |
|---------------|------------------------|
| • U_0 | U_{48n} |
| • U_1 | $U_{48min, unlimited}$ |
| • U_2 | $U_{48max, unlimited}$ |
| • t_0 | 100ms |
| • t_{r1} | 1ms |
| • t_1 | 1s |
| • t_r | 1s |
| • t_2 | 10s |
| • t_{f2} | 1s |
| • t_3 | 100ms |
| • Test case 1 | T_{min} |
| • Test case 2 | T_{RT} |
| • Test case 3 | T_{max} |
| • Test cycles | 10 |

E-16

Operation in the upper range with function limitation. The operating behavior with change and at the range limits is checked.

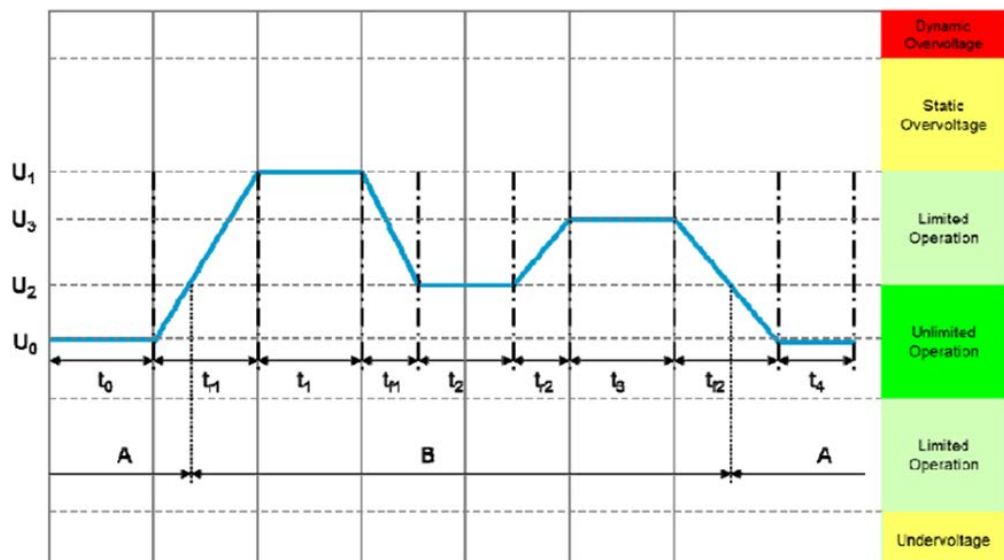


Test parameters:

| | |
|------------|------------------------------------|
| • U_0 | U_{48n} |
| • U_1 | $U_{48max,high,limited}$ |
| • U_2 | $U_{48max,unlimited}$ |
| • U_3 | $U_{48max,unlimited} + 1\text{ V}$ |
| • t_0 | 100ms |
| • t_{r1} | 4s |
| • t_1 | 10s |
| • t_{r1} | 2s |
| • t_2 | 10s |
| • t_{r2} | 2s |
| • t_3 | 10s |
| • t_4 | 100ms |

E-18 Overvoltage range

The test is to show the load cut-off during storage charging and check the changes of the operating behavior into the overvoltage range.

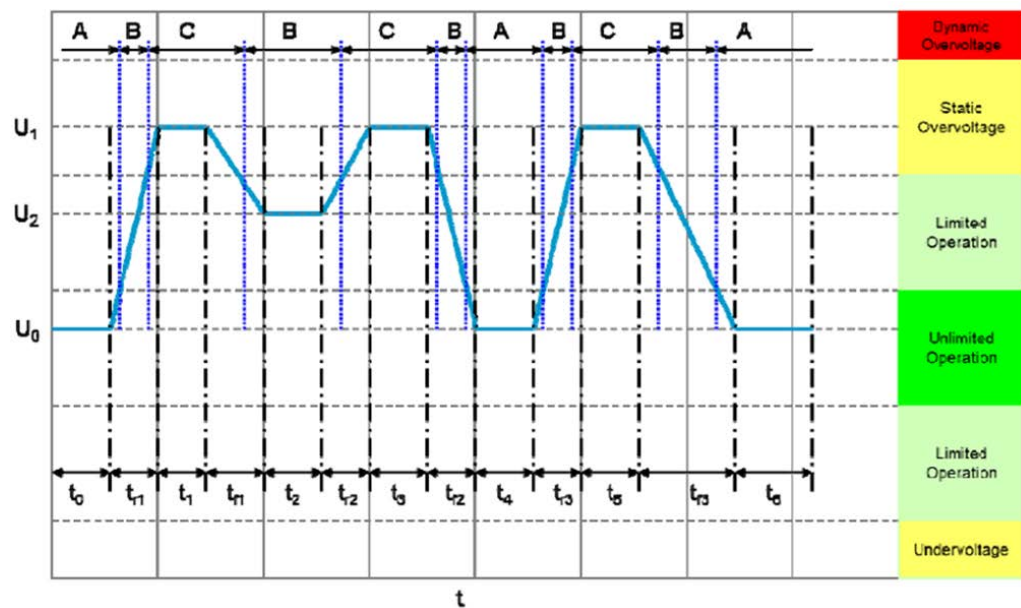

Test parameters:

| | |
|------------|-----------------------------|
| • U_0 | U_{48n} |
| • U_1 | U_{48r} |
| • U_2 | $U_{48max,unlimited} + 1 V$ |
| • t_0 | 100ms |
| • t_{r1} | 10ms |
| • t_1 | 1s |
| • t_{f1} | 1s |
| • t_2 | 10s |
| • t_{r2} | 1ms |
| • t_3 | 2s |
| • t_{f2} | 1s |
| • t_4 | 5s |
| • t_{r3} | 10s |
| • t_5 | 2s |
| • t_{f3} | 10s |
| • t_6 | 100ms |

How to Use

Take LV148 E-01a (long-term overvoltage test pulse) as an example to introduce how to use this function.


1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **LV148** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Testings** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **E-01a** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Testcase** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Standard** and press the **[Enter]** key to confirm.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.

4.7.8 ISO21780

TEST-01

The purpose of this test is to verify the component functionality in the nominal voltage range.

The waveform is as follows:

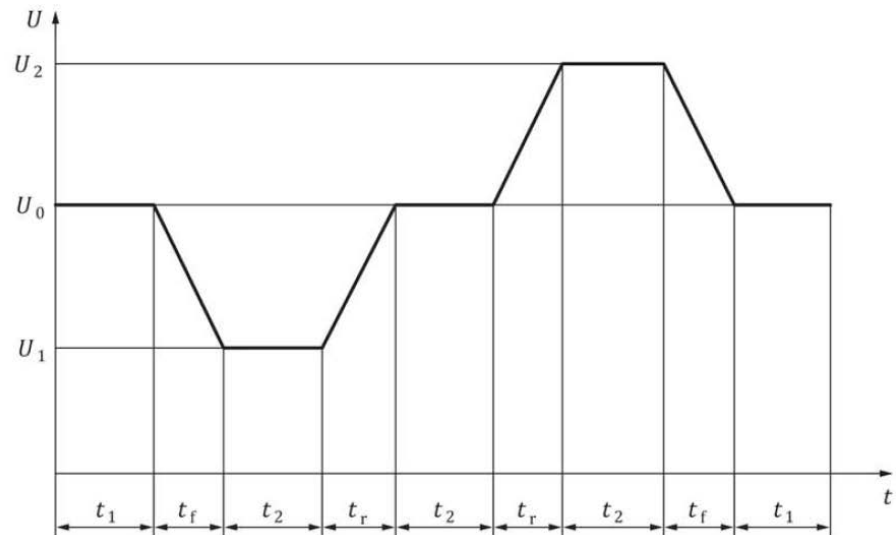
Key

t time


U test voltage

| | |
|------------------|-------------------|
| Operating mode | 2.4 |
| U_0 | 44 V |
| U_1 | 36 V |
| U_2 | 52 V |
| t_1 | 30 s |
| t_2 | 60 s |
| t_r | 50 ms (0,16 V/ms) |
| t_f | 50 ms (0,16 V/ms) |
| Number of cycles | 5 |

TEST-02

The purpose of this test is to verify the functionality of the component in the upper and lower transitory voltage range.

- The waveform of lower range is as follows:

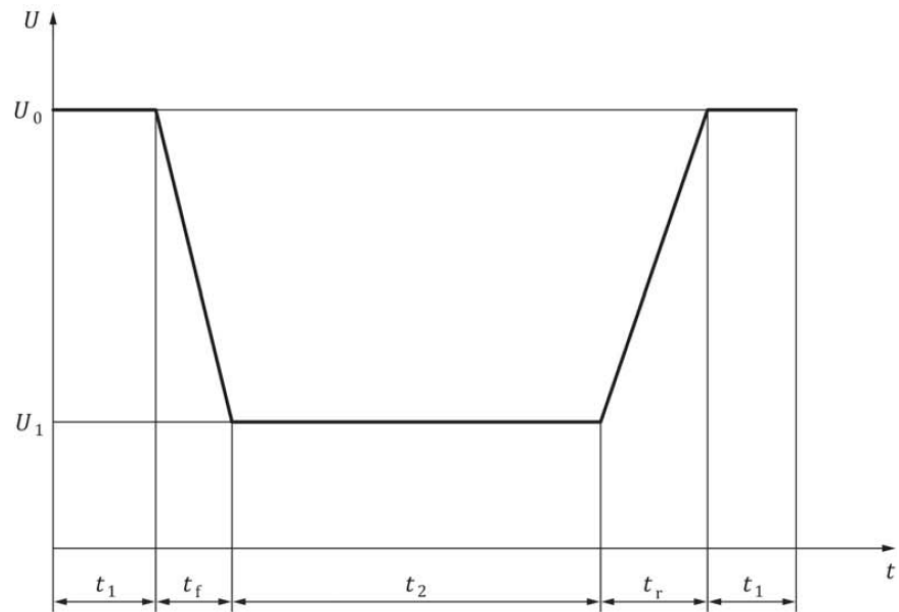

Key

t time

U test voltage

| | |
|------------------|------------------|
| Operating mode | 2.4 |
| U_0 | 36 V |
| U_1 | 31 V |
| t_1 | 60 s |
| t_2 | 2 s |
| t_r | 10 ms (0,5 V/ms) |
| t_f | 10 ms (0,5 V/ms) |
| Number of cycles | 5 |

- The waveform of upper range is as follows:

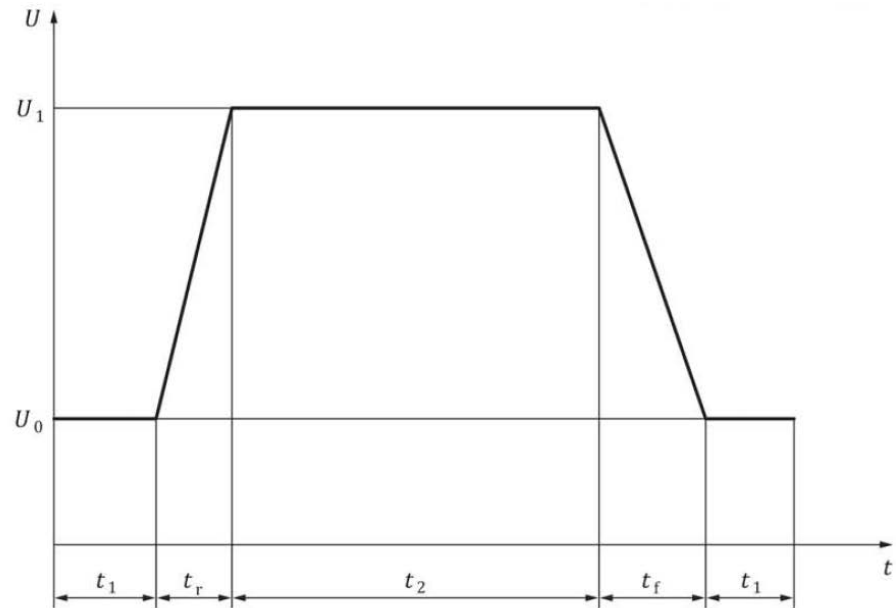
Key


t time

U test voltage

| | |
|------------------|-----------------|
| Operating mode | 2.4 |
| U_0 | 52 V |
| U_1 | 54 V |
| t_1 | 60 s |
| t_2 | 120 s |
| t_r | 4 ms (0,5 V/ms) |
| t_f | 4 ms (0,5 V/ms) |
| Number of cycles | 5 |

TEST-03

This test is intended to check the immunity of the component to transient overvoltages. The waveform is as follows:

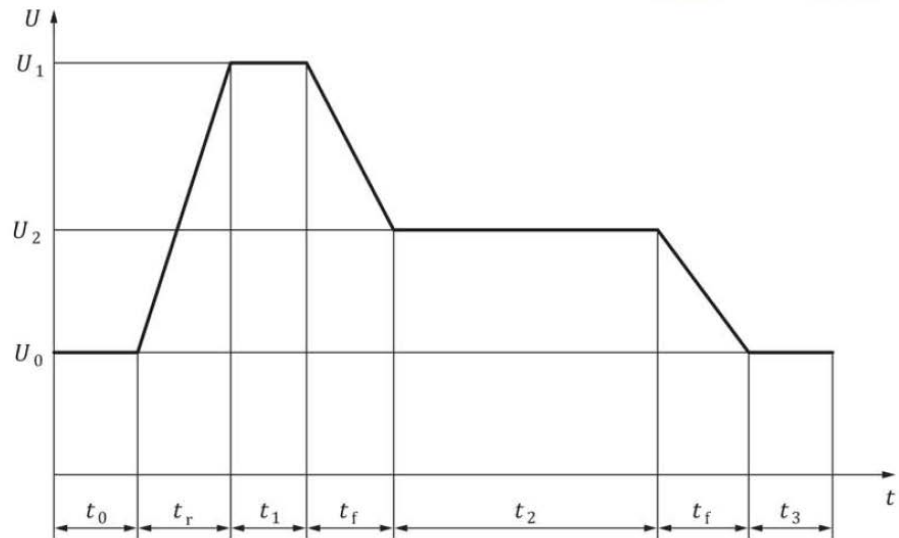
Key


t time

U test voltage

| | |
|------------------|---------------------|
| Operating mode | 2.4 |
| U_0 | 52 V |
| U_1 | 70 V |
| U_2 | 58 V |
| t_0 | ≥ 5 s |
| t_r | 0,7 ms (25,71 V/ms) |
| t_1 | 40 ms |
| t_f | 1 ms |
| t_2 | 600 ms |
| t_3 | ≥ 5 s |
| Number of cycles | 1 000 |

TEST-04

This test is a simulation of a load dump situation where voltage transients occur following a sudden reduction in the load current drawn from a generator, motorgenerator or DC/DC converter and whilst the battery is either out of circuit or incapable of absorbing power. The waveform is as follows:

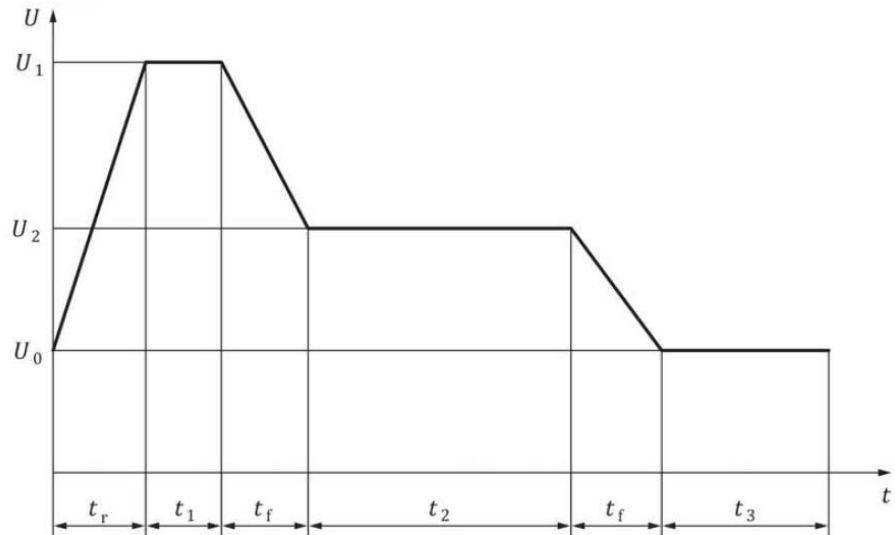
Key


t time

U test voltage

| | |
|----------------|--------|
| Operating mode | 2.4 |
| U_1 | 70 V |
| U_2 | 58 V |
| t_1 | 40 ms |
| t_2 | 600 ms |
| t_3 | 9 s |
| t_r | 0,7 ms |
| t_f | 1 ms |

TEST-05

This test is intended to check the immunity of the component to voltage variations during the cold crank phase. The waveform is as follows:

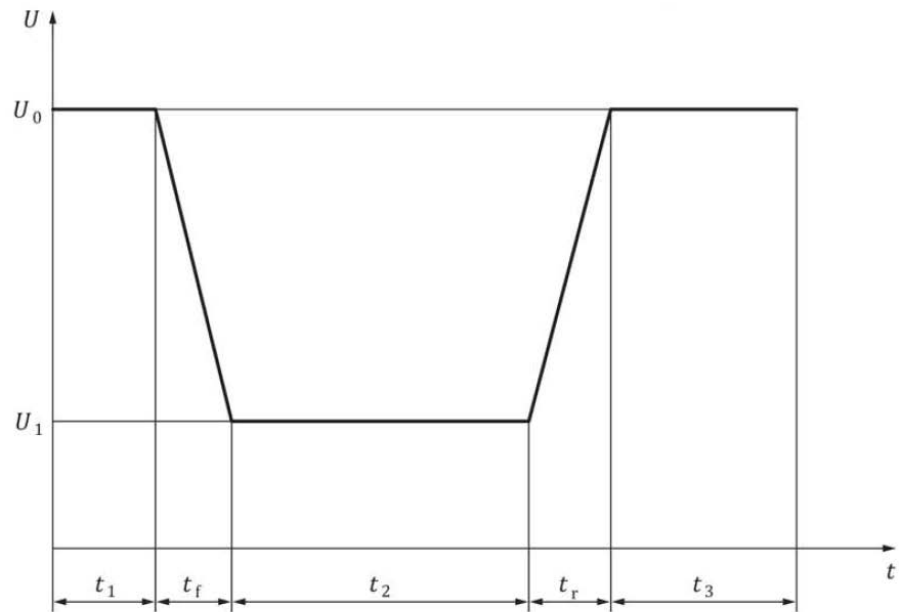


Key
t time
U test voltage

| | |
|------------------|------------------|
| Operating mode | 2.4 |
| U_0 | 36 V |
| U_1 | 24 V |
| t_f | 5 ms (2,4 V /ms) |
| t_2 | 10 s |
| t_r | 5 ms (2,4 V/ms) |
| t_1 | 2 s |
| t_3 | 60 s |
| Number of cycles | 10 |

TEST-06

This test checks the robustness of the component against a long-term overvoltage. The waveform is as follows:

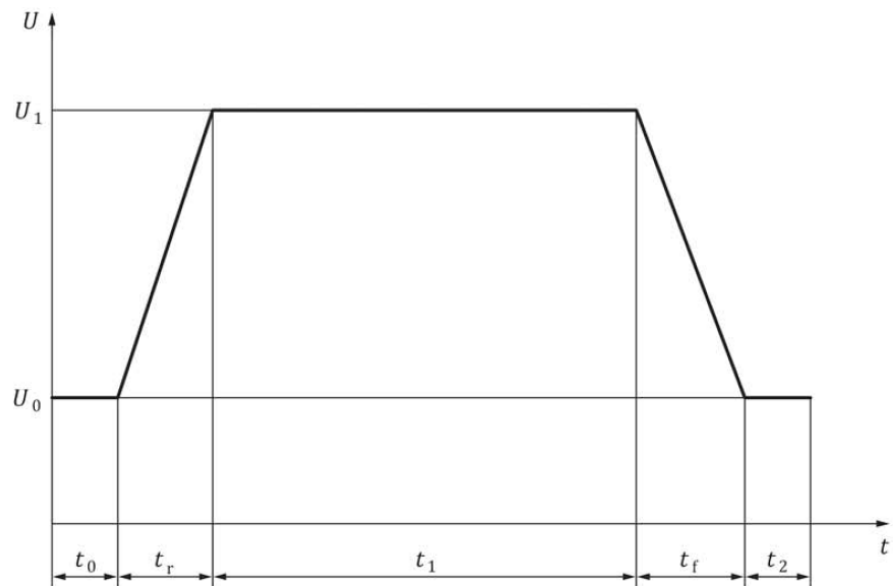
Key

t time

U test voltage

| | |
|-------------------|-------------------------|
| Operating mode | 2.4 |
| U_1 | 60 V |
| U_0 | 52 V |
| t_0 | ≥ 5 s |
| t_r | 0,1 s (80 V/s) |
| t_1 | 60 min |
| t_f | 0,1 s (80 V/s) |
| t_2 | ≥ 5 s |
| T_{test} | $T_{\text{max}} - 20$ K |
| Number of cycles | 1 |

TEST-07

This test is applicable to all components which not only consume electrical energy but may also supply electrical energy with no possibility of switching off this electrical energy supply without negative effects occurring in the vehicle.


Such components shall either be capable of self-limiting their output supply voltage or systematic countermeasures shall be applied to the vehicle in order to ensure compliance with this specification.

This test does not apply to components that supply electrical energy as a primary function, such as generators. For these components TEST-04 is applicable.

The purpose of this test is to verify that the component alone complies with the voltage range specified here and is applicable where systematic countermeasures at the vehicle level are not used to ensure compliance.

The test emulates a condition where such a component supplies energy into the vehicle 48 V power supply system which can only be absorbed by the power network simulation and subsequently leads to an undesired increase in system voltage.

The waveform is as follows:

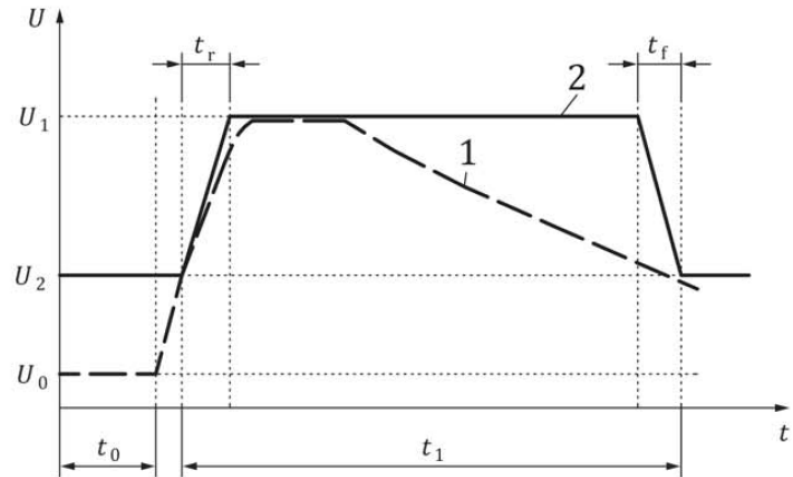


Key

- t time
- U test voltage
- 1 example of the test result of the component
- 2 limit

| | |
|-------|---------------------------------|
| U_1 | 58 V |
| U_2 | 54 V |
| t_r | $\geq 160 \mu\text{s}$ (25V/ms) |
| t_f | $\geq 160 \mu\text{s}$ (25V/ms) |
| t_1 | 300 ms |

TEST-08

This test is intended to check immunity of a component to decrease and increase of supply voltages. The waveform is as follows:

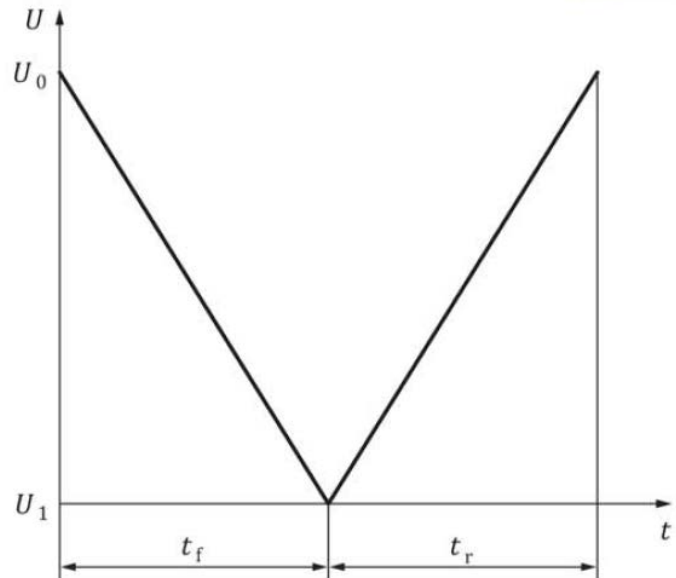
Key


t time

U test voltage

| | |
|------------------|-----------------------------|
| Operating mode | 2.1 and 2.4 |
| U_0 | 44 V |
| U_1 | 0 V |
| t_f | 21 min (≈ 35 mV/s) |
| t_r | 21 min (≈ 35 mV/s) |
| Number of cycles | 1 |

TEST-10

This test is intended to check the correct reinitialisation of the component after interruption of onboard power supply. This test shall only be performed on DUT's whose control logic (or parts thereof) is supplied by 48 V. The waveform is as follows:

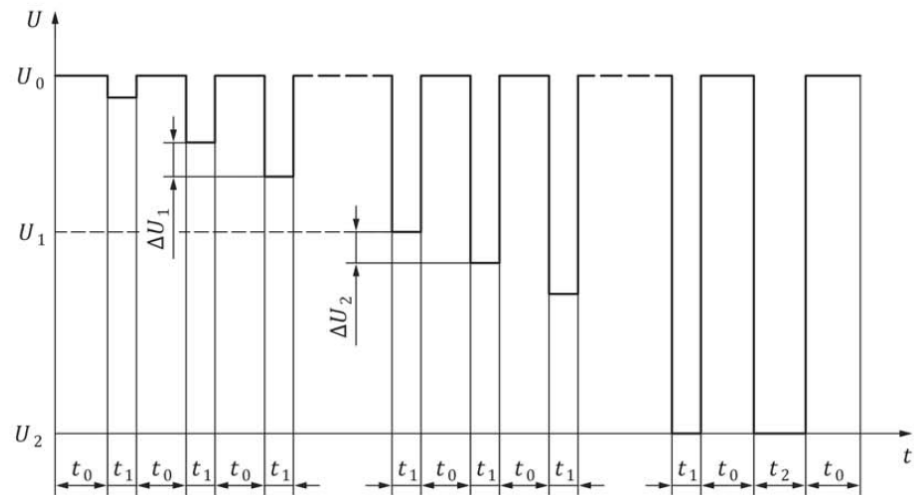
Key

t time
 U test voltage


| | |
|----------------|--|
| Operating mode | 2.4 |
| U_0 | 36 V |
| U_1 | 24 V |
| U_2 | 0 V |
| ΔU_1 | 2 V |
| ΔU_2 | 0,5 V |
| t_f | <100 ms |
| t_r | <100 ms |
| t_1 | 5 s |
| t_2 | 10 s |
| t_0 | ≥ 10 s, until the DUT becomes 100 % operational |

TEST-11

The behaviour of a component when subjected to interruption of supply of varying duration is tested. Examples for this occurrence may be short circuits, switching of loads, disconnecting of batteries and others.


This test applies to power consumers and not to power generators.

The waveform is as follows:

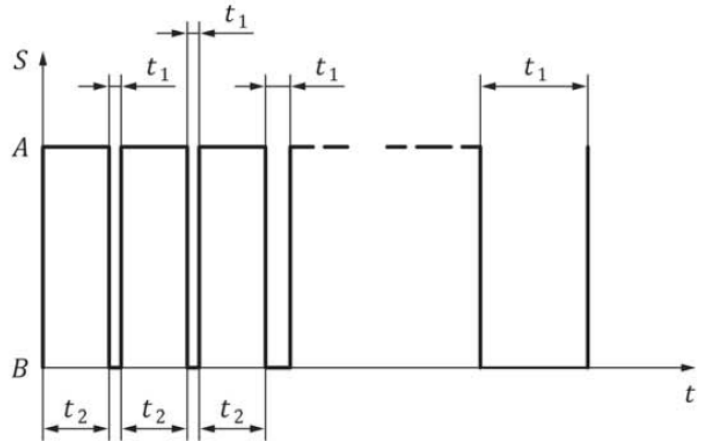
Key

- t time
 S S_1 switch control signal
 A switch closed
 B switch open

| | | |
|----------------------|---|--|
| Operating mode | 2.3 and 2.4 | |
| R_i | $\leq 60 \text{ m}\Omega$ incl. switch S_1 | |
| U_0 | 48 V | |
| t_1 | The supply voltage of U_0 is interrupted for interval t_1 , which shall increase during the test in the following sequence: | |
| | Range of t_1 | Increment in t_1 following each interruption |
| | $100 \mu\text{s} \leq t_1 < 1 \text{ ms}$ | 100 μs |
| | $1 \text{ ms} \leq t_1 < 10 \text{ ms}$ | 1 ms |
| | $10 \text{ ms} \leq t_1 < 100 \text{ ms}$ | 10 ms |
| | $100 \text{ ms} \leq t_1 < 2 \text{ s}$ | 100 ms |
| t_2 | $\geq 10 \text{ s}$, until the DUT becomes 100 % operational according to specification | |
| switch reaction time | $\leq 10 \mu\text{s}$ | |

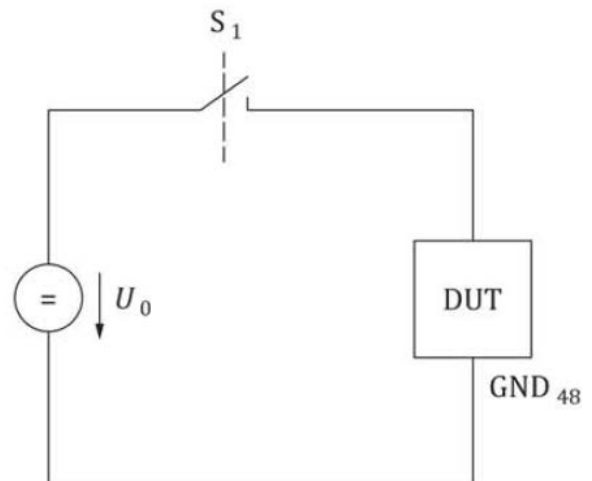
Key

- S_1 switch on 48 V supply

How to Use


Take ISO21780 TEST-01 as an example to introduce how to use this function.

1. Click Vehicle on the Menu screen to enter the vehicle test screen.
 - 1) Press the up/down key to move the cursor to the **Standards** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **ISO21780** and press the **[Enter]** key to confirm.
 - 2) Press the up/down key to move the cursor to the **Testings** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **TEST-01** and press the **[Enter]** key to confirm.
 - 3) Press the up/down key to move the cursor to the **Testcase** function setting and press the **[Enter]** key to confirm. Rotate the knob to select **Standard** and press the **[Enter]** key to confirm.
2. Press **[Run]** in the Vehicle function interface.
3. Press **[On/Off]** on the front panel, turn on the output.
4. According to the selected trigger method, for example, press **[Shift]+[5]**(Trigger) to trigger the output of the waveform.

4.7.9 ISO21498-2


ISO21498-2 covers electrical specifications and tests for voltage class B systems and components. The component voltage range and limits of corresponding OS are shown in the figure below.

In the ISO21498-2 main interface, by clicking on "More" you can access the settings menu to adjust different voltage ranges.

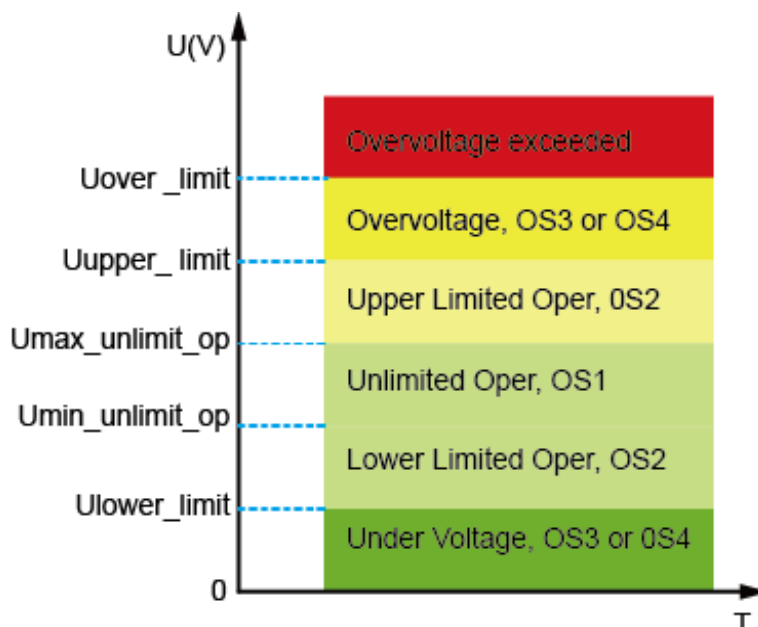

E-04


This test verifies that the DUT is able to perform as specified when the DC voltage varies in the range between the lower voltage limit and the upper voltage limit.

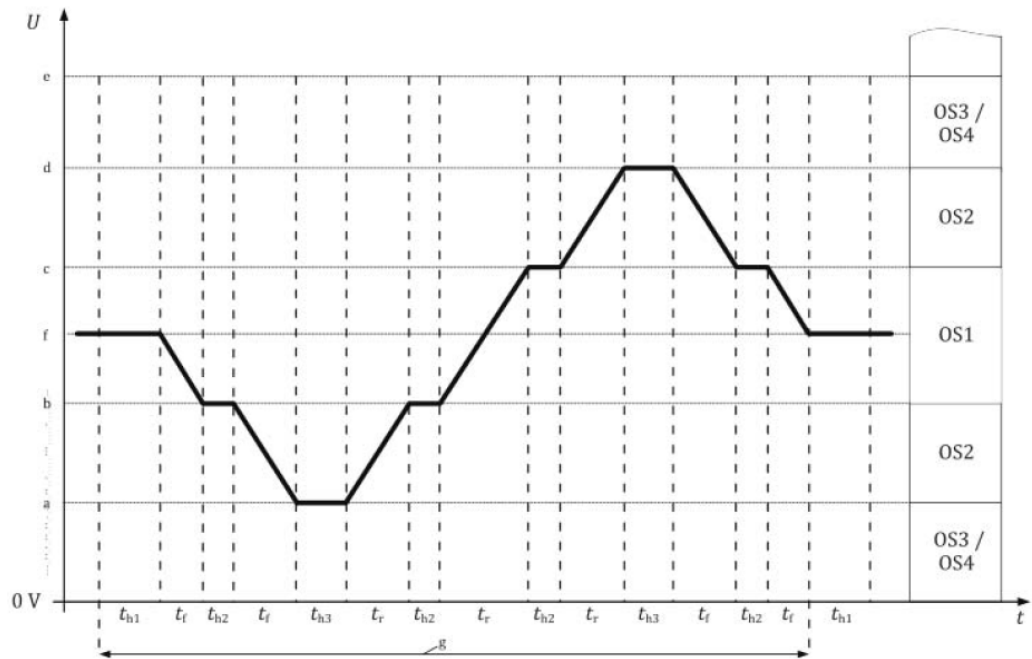

| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Ua | 60V |
| Ub | 90V |
| Uf | 140V |
| Uc | 190V |
| Ud | 220V |
| th1 | $\geq 30s$ |
| th2 | $\geq 5s$ |
| th3 | $\geq 10s$ |

E-06

This test evaluates the generated voltage slope and confirms that it is within a specified maximum rate.

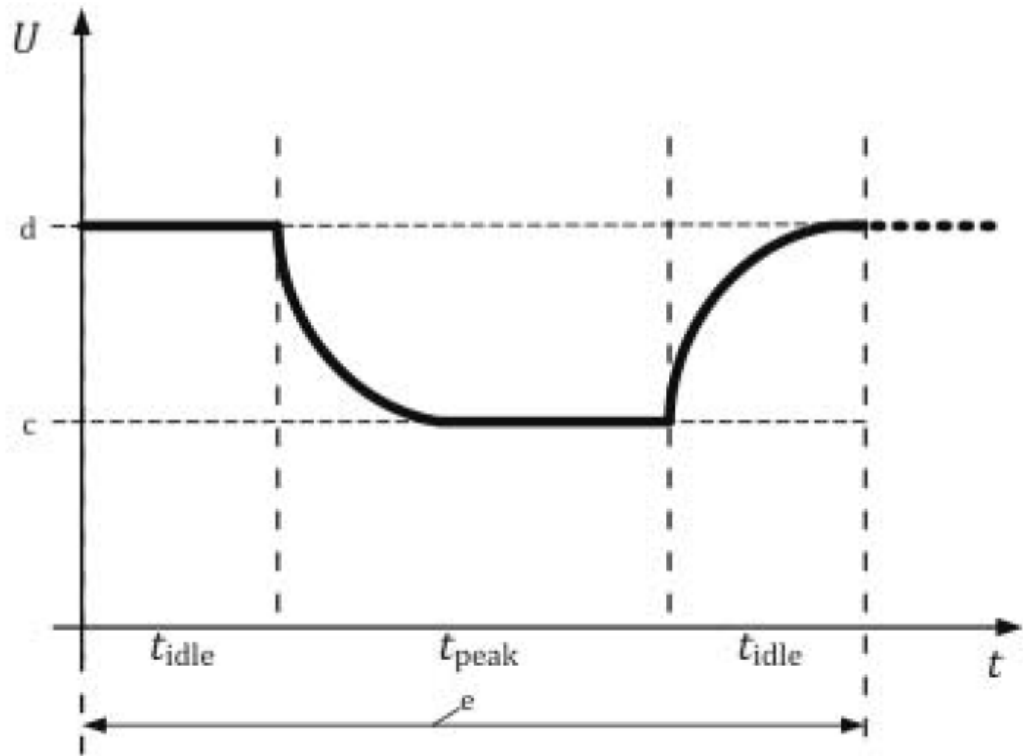


| Parameter | Description |
|-------------------|-------------|
| Ranges | B_220 |
| Uc | 90V |
| Ud | 190V |
| t _{idle} | 10s |
| t _{peak} | 2s |
| cycles | 10 |

E-08


This test simulates a voltage slope at the power input of the component to verify its robustness. It shall be verified that the voltage class B operating status of the component in the respective operating voltage range does not change due to voltage slope present in the voltage class B circuit and that the component is able to provide the corresponding performance.

- E-08a

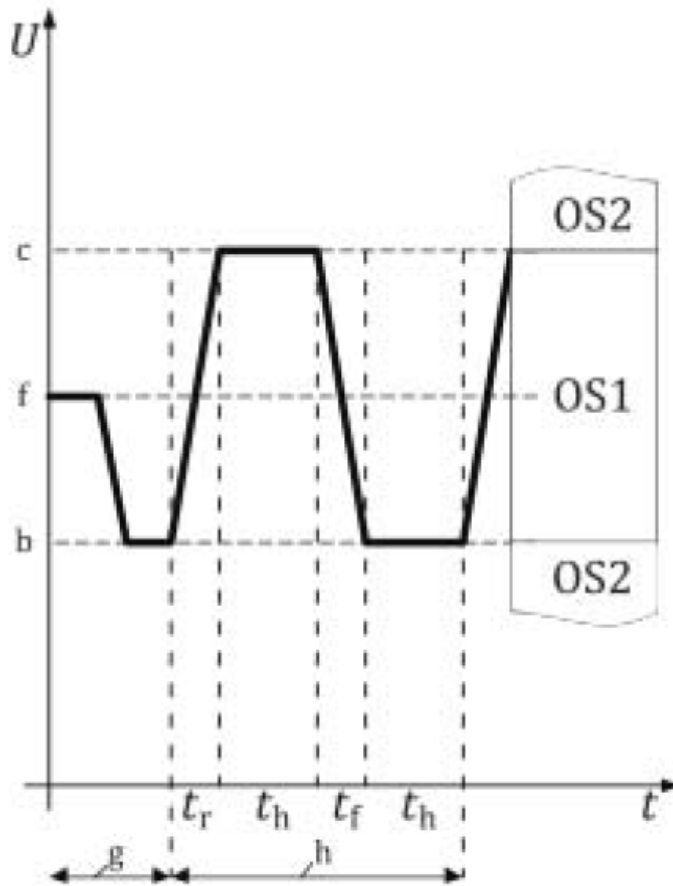


| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Ub | 90V |
| Uf | 140V |
| Uc | 190V |
| th | $\geq 2s$ |
| tr | 10V/ms |
| tf | 10V/ms |
| cycles | 3 |

- E-08b

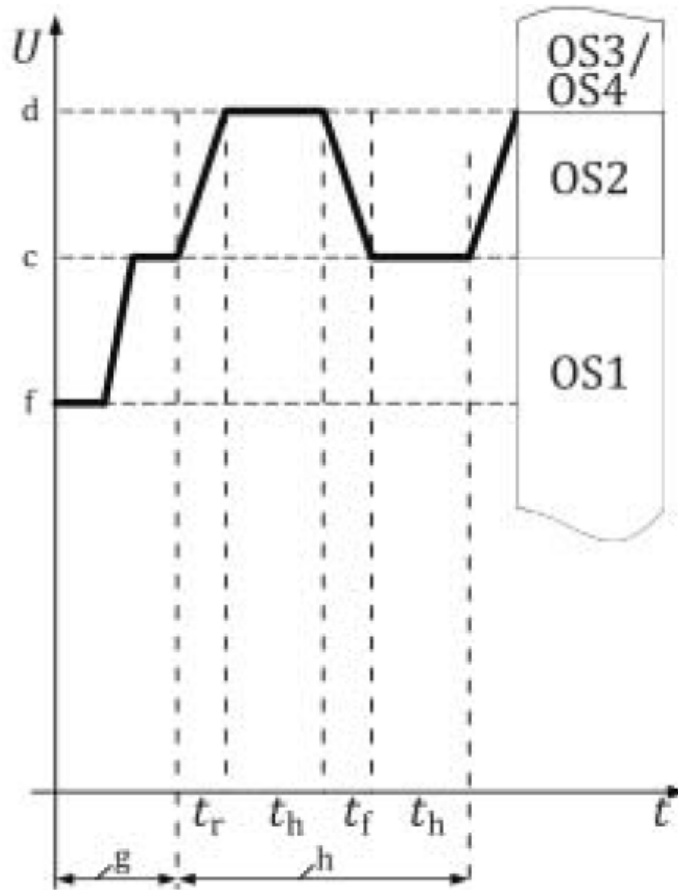

| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Uf | 140V |
| Uc | 190V |
| th | >=2s |
| tr | 10V/ms |
| tf | 10V/ms |
| cycles | 3 |


- E-08c

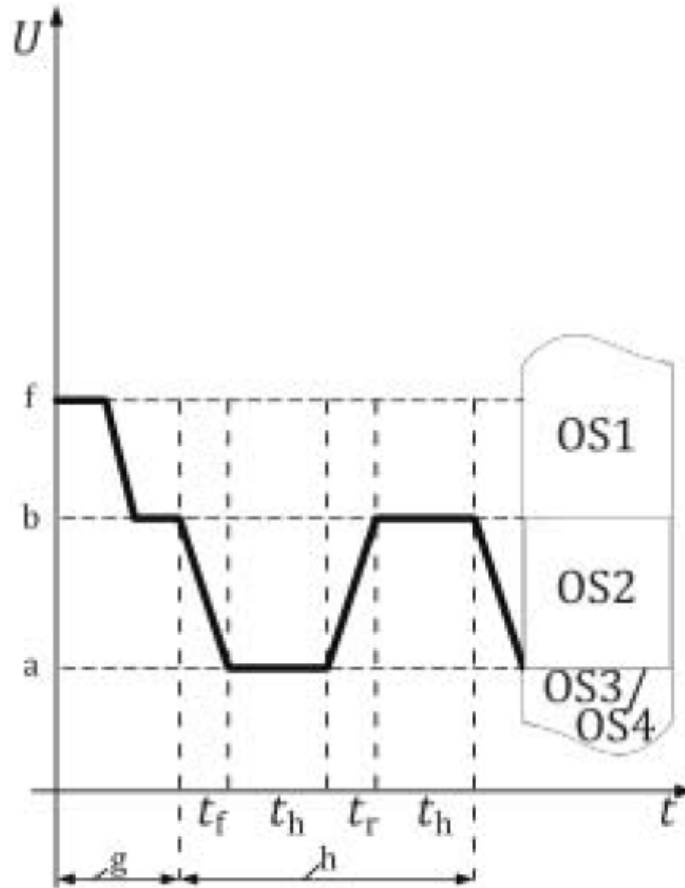

| Parameter | Description |
|-----------|---------------|
| Ranges | B_220 |
| Ua | 60V |
| Ub | 90V |
| Uf | 140V |
| th | $\geq 0.001s$ |
| tr | 10V/ms |
| tf | 10V/ms |
| cycles | 1 |

E-16


This test evaluates the component's robustness in case the DC voltage rises above the upper voltage limit. The test verifies if the component is able to protect itself or withstand a specified maximum voltage limit within the overvoltage limit.

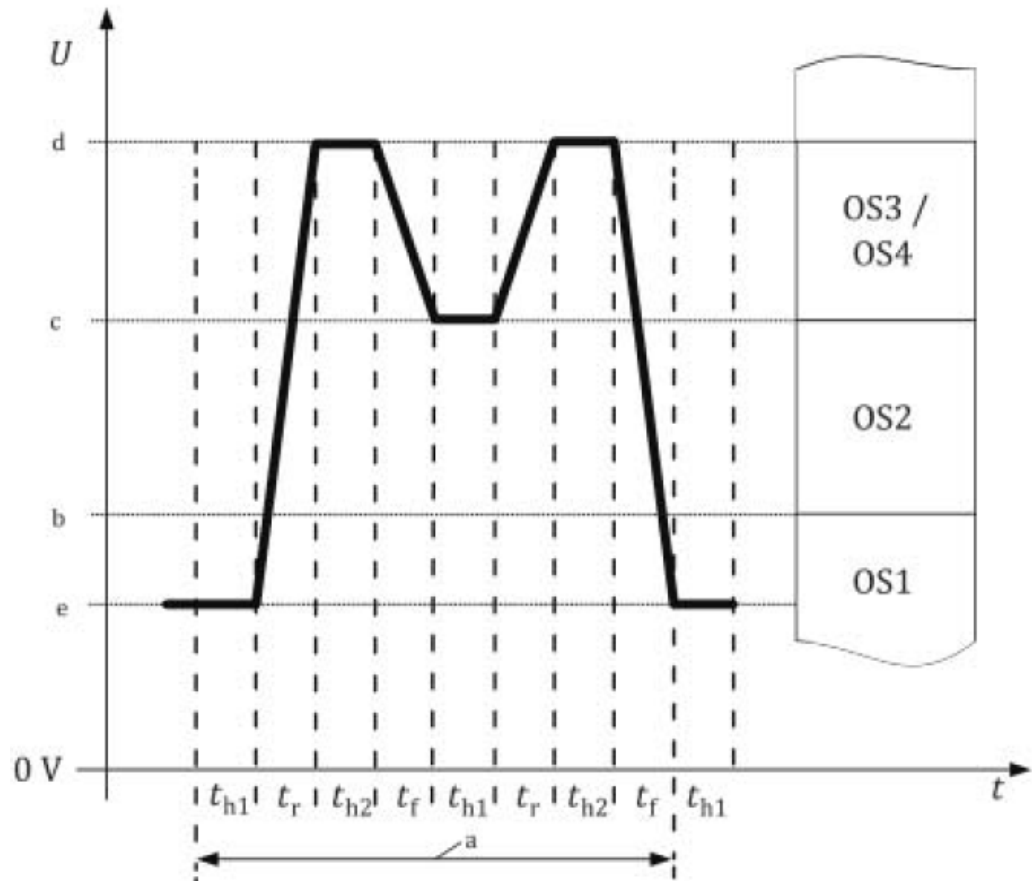

| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Ue | 140V |
| Uc | 220V |
| Ud | 250V |
| th1 | 30s |
| th2 | 10s |
| tr | 2V/s |
| tf | 2V/s |
| cycles | 10 |

E-18

This test evaluates the component's robustness in case the DC voltage drops below the lower voltage limit. The test verifies if the DUT is able to perform correctly during an undervoltage event.

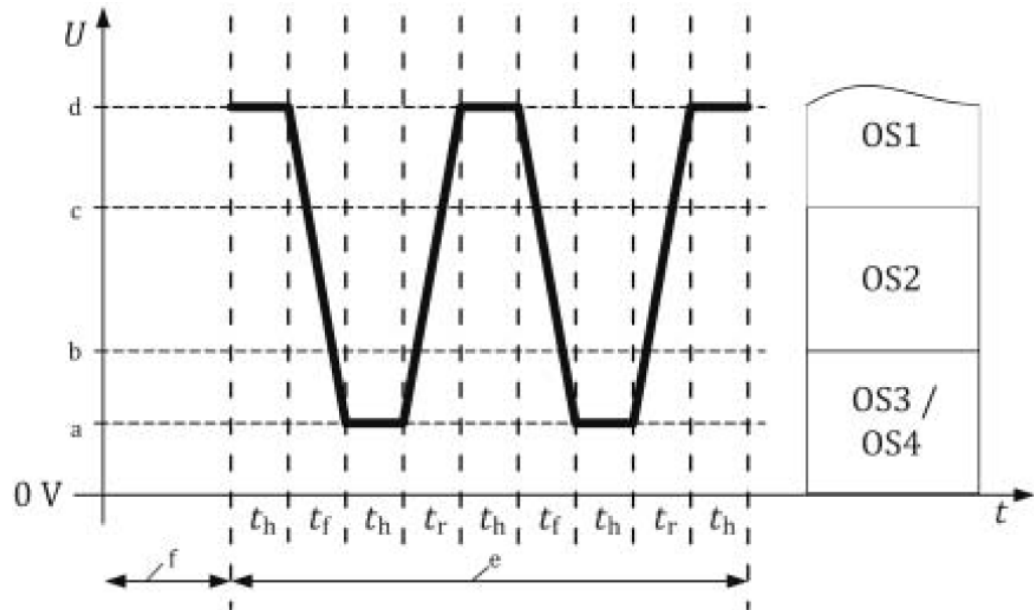


| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Ua | 30V |
| Ud | 140V |
| th | 20s |
| tr | 2V/s |
| tf | 2V/s |
| cycles | 5 |

E-21

This test evaluates the DUT's robustness in case that the isolation resistance to ground reference decreases.


This test covers the worst-case condition which is the electrical connection of one of the two power lines to the ground reference.

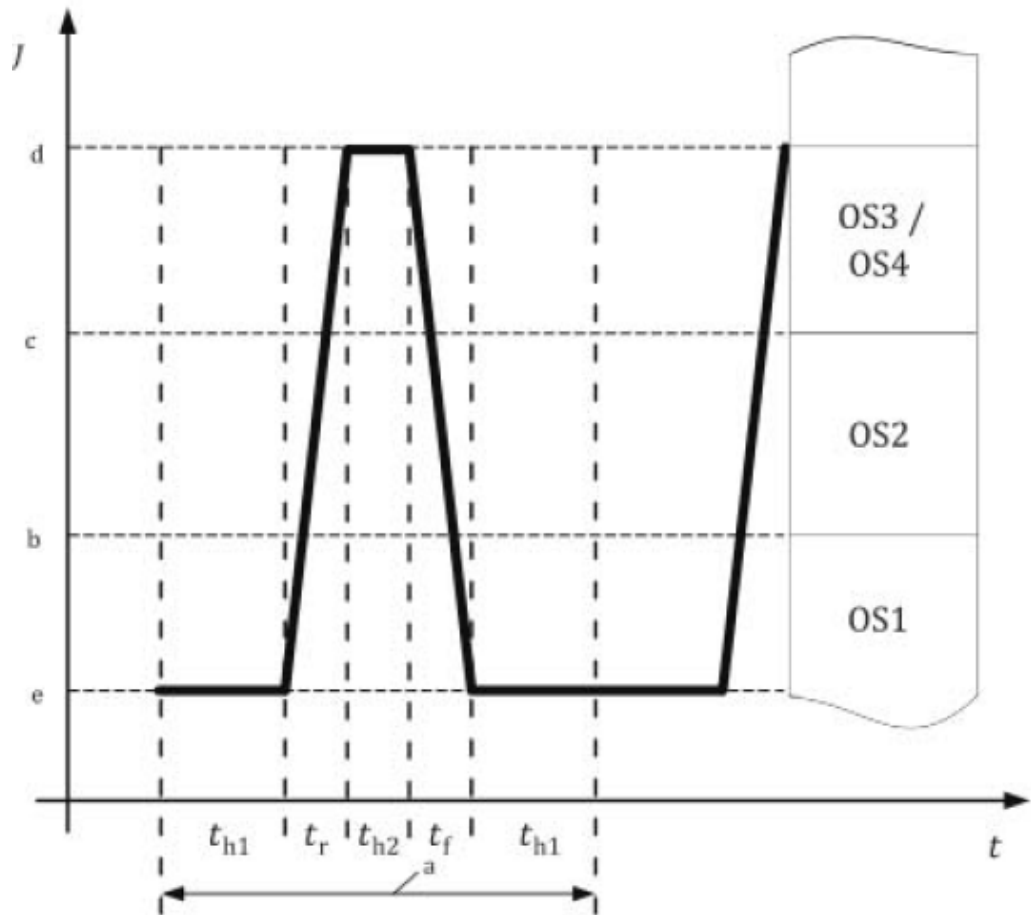

| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Ue | 140V |
| Ud | 250V |
| th1 | 30s |
| th2 | 10s |
| tr | 2V/s |
| tf | 2V/s |
| cycles | 1 |

E-23


This test verifies if a voltage class B component is able to limit the overvoltage during a load dump.

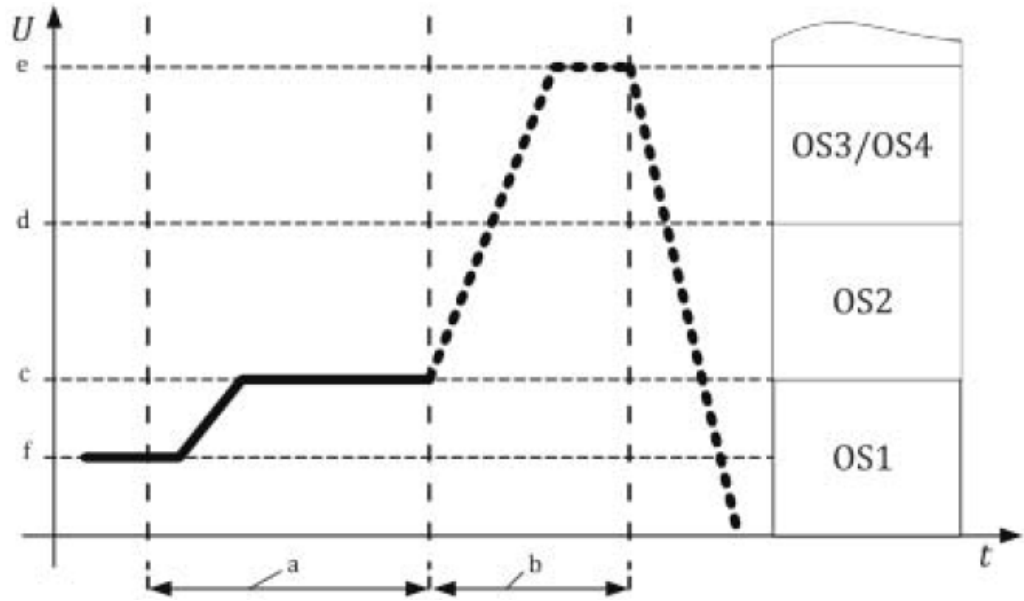

| Parameter | Description |
|-----------|-------------|
| Ranges | B_220 |
| Uf | 140V |
| Uc | 190V |
| Ud | 250V |

E-25

This test verifies if a voltage class B component is able to withstand the fast voltage rise and the overvoltage caused by a load dump.

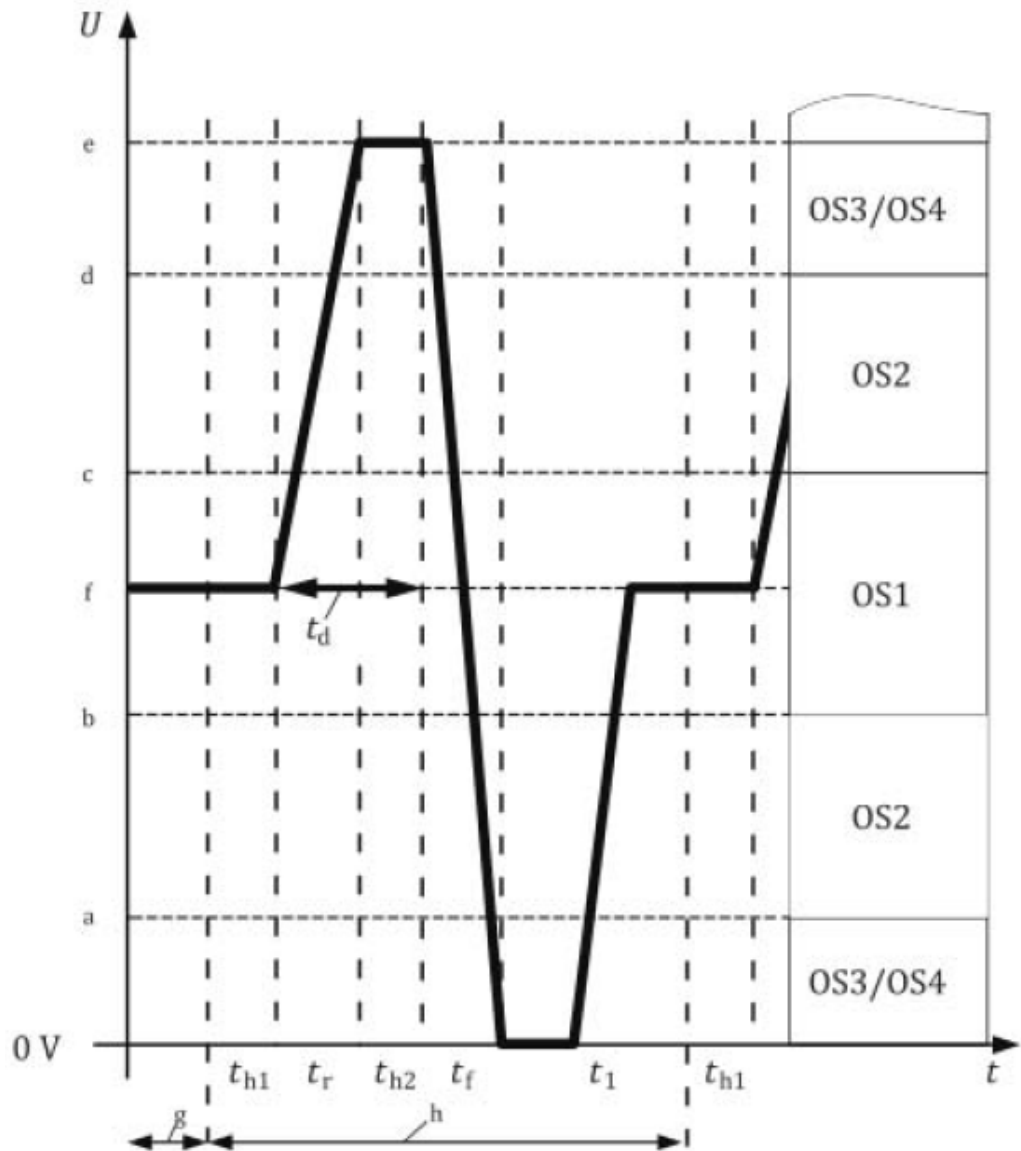

| Parameter | Description |
|-----------------|-------------|
| Ranges | B_220 |
| U _f | 140V |
| U _e | 250V |
| t _{h1} | 30s |
| t _{h2} | 30s |
| t _r | 250V/ms |
| t _f | 250V/ms |
| t ₁ | 30s |
| cycles | 5 |

4.8 Standard IEC Regulations

IT6600 series power supplies provide standard test curves in accordance with IEC 61000-4-17/4-29 regulations. It can be invoked directly by the user when testing IEC compliance tests.

This function provides both the test curve that meets the standard requirements of regulations and the curve customization function. Users can customize the curve according to the project requirements of regulations and perform the extended test of the test object.

Click IEC on the Menu screen to enter the regulation test screen.




NOTE

For parameters of corresponding curves and related regulations, refer to IEC standards.

4.8.1 IEC 61000-4-17

Interface Instruction

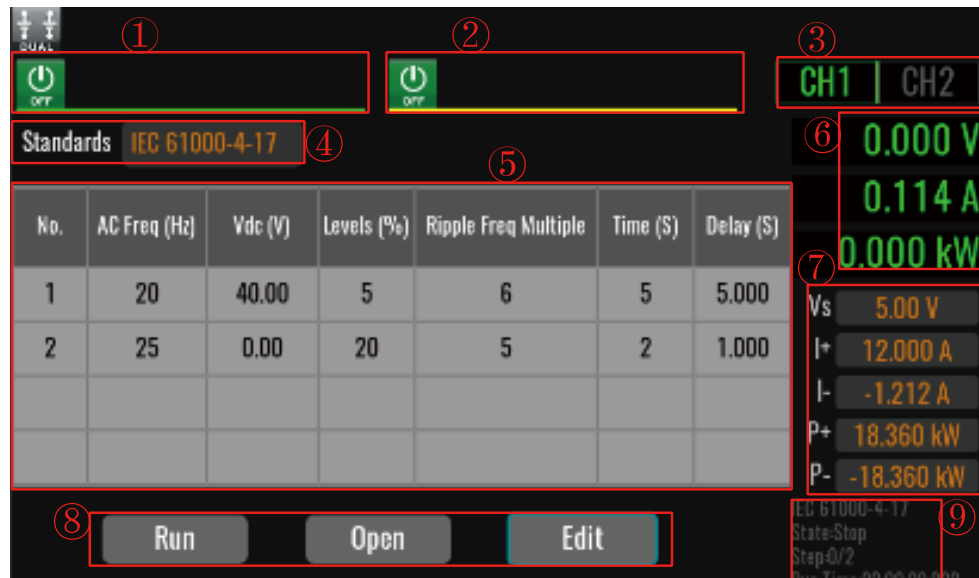

1. CH1 status bar: displays the output status of power channel 1.
2. CH2 status bar: displays the output status of power channel 2.
3. CH1/CH2: channel selection, Channel 1 or Channel 2.
4. Standards: the current supporting regulation is IEC 61000-4-17/4-29.
5. Display area: this area mainly displays the edited IEC, you can view this IEC by sliding up and down.
6. Output values view area: displays the output voltage value, output current value and output power value of the current channel.
7. Setting values view area (Normal mode): When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.
8. IEC edit button. The functions are described as follows.
 - Run/Stop: run/stop the IEC function.
 - Open: select the IEC file to execute.
 - Edit: edit present IEC file.
9. Displays the IEC function relevant parameters, which can be viewed by

sliding up and down.

Edit IEC files

1. Click IEC on the Menu screen to enter the regulation test screen.
2. Click the **[Edit]** key on the screen and enter to the IEC file edit interface.



| No. | AC Freq (Hz) | Vdc (V) | Levels (%) | Ripple Freq Multiple | Time (S) | Delay (S) |
|-----|--------------|---------|------------|----------------------|----------|-----------|
| 1 | 20 | 40.00 | 15 | 5 | 4 | 3.000 |
| 2 | 25 | 30.00 | 20 | 6 | 2 | 1.000 |
| 3 | | | | | | |

IEC parameters description:

| | |
|----------------------|---|
| AC Freq [Hz] | Frequency setting value. |
| Vdc [v] | Voltage value of DC output. User can setting the voltage level according to the DUT requirements. |
| Levels [%] | Percentage of the nominal dc voltage. |
| Ripple Freq Multiple | Ripple freq multiple. |
| Time [s] | Test time. |
| Delay [s] | Time delay, the time interval between test items. |
| Save | Save the IEC file. |
| Config | Configure the IEC file to make it effective. |
| Clear all | Delete all of step information. |

3. Fill in corresponding parameter in the IEC file edit interface and press **[Save]**.
4. Press **[Esc]**, and return to the IEC function interface. The IEC display zone displays the edited IEC file.


Select/Run IEC File

If several IEC files are edited, press **Open** to recall the IEC file to be tested. Detailed operation steps are as below:

1. Click IEC on the Menu screen to enter the regulation test screen.
2. Click the **[Open]** key on the screen, select the saved .csv file, and click the **[Open]** key to enter the file.
3. Press **[On/Off]** on the front panel, turn on the output.
4. Press **[Run]** key in the IEC function interface to run the IEC file.
Click **[Stop]** to stop the present running.

4.8.2 IEC 61000-4-29

Interface Instruction

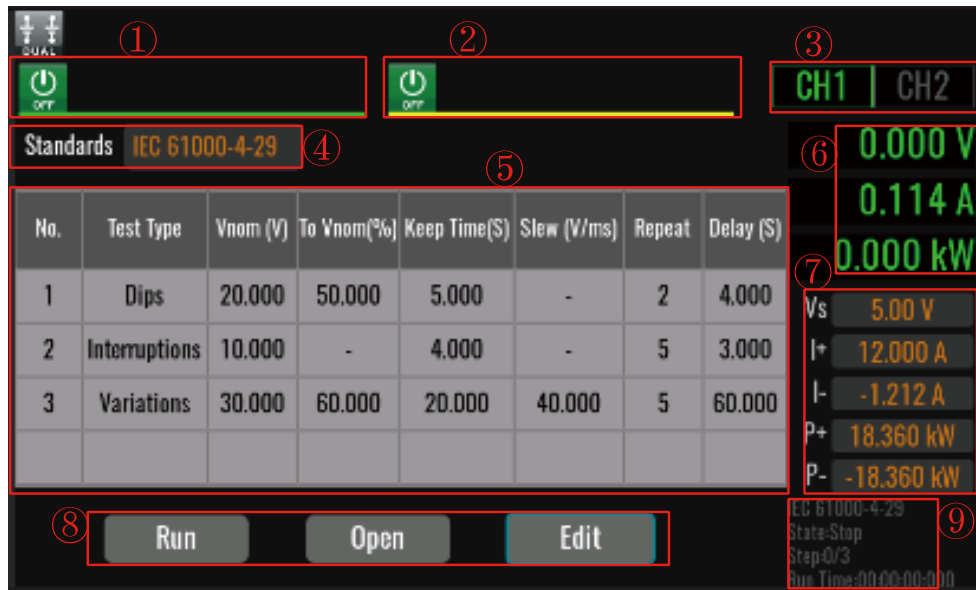

1. CH1 status bar: displays the output status of power channel 1.
2. CH2 status bar: displays the output status of power channel 2.
3. CH1/CH2: channel selection, Channel 1 or Channel 2.
4. Standards: the current supporting regulation is IEC 61000-4-17/4-29.
5. Display area: this area mainly displays the edited IEC, you can view this IEC by sliding up and down.
6. Output values view area: displays the output voltage value, output current value and output power value of the current channel.
7. Setting values view area (Normal mode): When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.
8. IEC edit button. The functions are described as follows.
 - Run/Stop: run/stop the IEC function.
 - Open: select the IEC file to execute.
 - Edit: edit present IEC file.
9. Displays the IEC function relevant parameters, which can be viewed by sliding up and down.

Edit IEC files

1. Click IEC on the Menu screen to enter the regulation test screen.
2. Click the **[Edit]** key on the screen and enter to the IEC file edit interface.

| IEC Edit | | | | | | | CH1 |
|---|---------------|----------|-------------|---------------|-------------|--------|-----------|
| File Name: Untitled-02.csv IEC 61000-4-29 | | | | | | | |
| No. | Test Type | Vnom (V) | To Vnom (%) | Keep Time (S) | Slew (V/ms) | Repeat | Delay (S) |
| 1 | Dips | 20.000 | 50.000 | 5.000 | - | 6 | 1.000 |
| 2 | Interruptions | 45.000 | - | 5.000 | - | 5 | 1.000 |
| 3 | Variations | 36.000 | 40.000 | 4.000 | 6.000 | 8 | 5.000 |
| 4 | | | | | | | |
| | | | | | | | |

Save Config Clear All

IEC parameters description:

| | |
|---------------|--|
| Test Type | Select the test type. <ul style="list-style-type: none"> ● Dips: Voltage dips. ● Interruptions: Short interruptions. ● Variations: Voltage variations. |
| Vnom [V] | The rated voltage of the device under test. |
| To Vnom [%] | Set the test level. |
| Keep Time [s] | Test time. |
| Slew [V/ms] | Voltage change slew. |
| Repeat | Repeat number. |
| Delay [s] | Time delay, the time interval between test items. |
| Save | Save the IEC file. |
| Config | Configure the IEC file to make it effective. |
| Clear all | Delete all of step information. |

3. Fill in corresponding parameter in the IEC file edit interface and press **[Save]**.
4. Press **[Esc]**, and return to the IEC function interface. The IEC display zone displays the edited IEC file.

Select/Run IEC File

If several IEC files are edited, press **Open** to recall the IEC file to be tested. Detailed operation steps are as below:

1. Click IEC on the Menu screen to enter the regulation test screen.
2. Click the **[Open]** key on the screen, select the saved .csv file, and click the **[Open]** key to enter the file.
3. Press **[On/Off]** on the front panel, turn on the output.
4. Press **[Run]** key in the IEC function interface to run the IEC file.
Click **[Stop]** to stop the present running.

4.9 Solar Photovoltaic Curve Simulation Function (SAS)

The IT6600 series power supply provides the maximum power point tracking (MPPT) mechanism built-in, and it is very important to test the efficiency of this MPPT. The PV array/module/cell is a device that converts from light energy to

electric energy. It is made by a simple semiconductor PN junction that the major output characteristic is that there's only one maximum power point (MPP) at certain sunlight intensity. The PV inverter is designed to track this point to harvest maximum energy that is generated by the PV array.

Introduction of SAS interface



1. CH1 status bar: displays the output status of power channel 1.
2. CH2 status bar: displays the output status of power channel 2.
3. CH1/CH2: channel selection, Channel 1 or Channel 2.
4. SAS edit button. The functions are described as follows.
 - Download: Download the SAS configuration to make it effective.
 - Run/Stop: Run/stop the SAS function.
 - Open: Select the PV curve file to execute.
 - Edit: Edit present PV curve file.
5. PV analog output in Userdefined mode. Support setting Voc, Vmp, Imp and Isc parameters.
6. Output values view area: displays the output voltage value, output current value and output power value of the current channel.
7. Setting values view area: When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.
8. PV Curve
9. Displays the relevant parameters of the PV curve file.
 - File name: the PV curve file name to execute.
 - Mode: edit mode of the PV curve.
 - MPPT: maximum power point tracking.

Edit Static PV Curve


IT6600 series power supplies provide both Userdefined and Curve for the user

to edit PV curves.

- **Curve**

You can edit the static PV curve and save it inside the instrument, the steps to edit a static curve locally on the instrument are as follows:

1. Click SAS on the Menu screen to enter the SAS function main interface.
2. Press **[Edit]** and enter to the PV curve file edit interface.

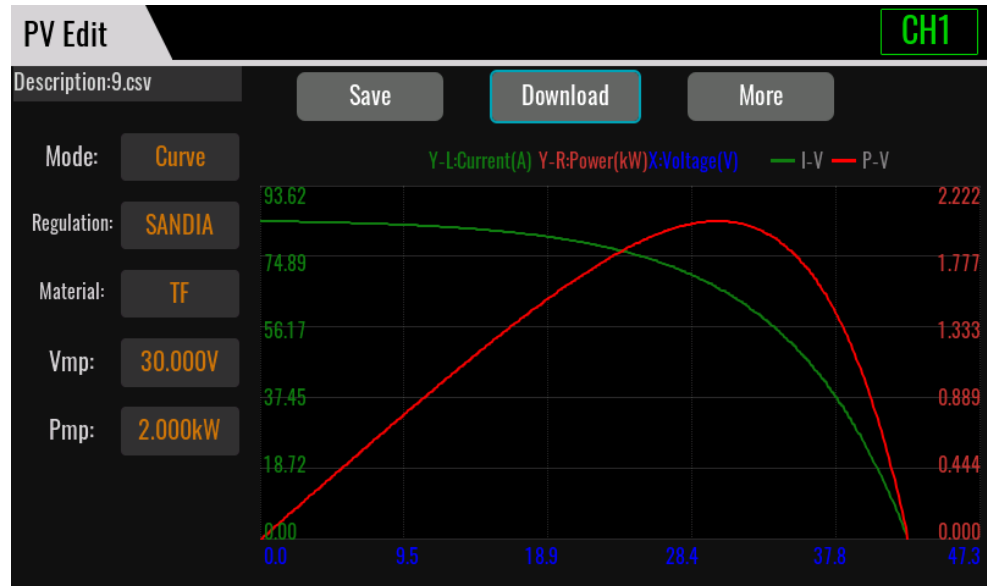

PV edit description:

| Parameter | Description |
|-------------|--|
| Description | Display PV curve file name. |
| Mode | Select the PV curve working mode User-defined or Curve. |
| Regulation | There are two regulation items for setting: <ul style="list-style-type: none"> ● EN50530 ● SANDIA |
| Material | Set solar panel material. Materials are different under different regulation item. <p>EN50530</p> <ul style="list-style-type: none"> ● TF: Thin-Film ● CSi <p>SANDIA</p> <ul style="list-style-type: none"> ● TF: Thin-Film ● SCMC: Standard Crystalline or Multi-crystalline ● HEC:High Efficiency Crystalline |
| Vmp | Voltage of maximum power. |
| Pmp | Maximum power |
| Save | Save the PV curve file. |
| Download | Download the SAS configuration to make it effective. |


| Parameter | Description |
|-----------|--|
| More | <ul style="list-style-type: none"> ● Filter: Filter the voltage collected from the output terminals of this instrument to reduce interference factors. Low(Low Speed Filtering), Mmedium(Medium Speed Filtering), High(High Speed Filtering). ● Priority: Sets the output priority mode, CC or CV. ● Sas Speed: When CC is prioritized, the current loop speed is set; when CV is prioritized, the voltage loop speed is set. |

3. Fill in corresponding parameter in the PV edit interface. Click **[More]** enter to advanced menu of PV file.
4. Press **[Esc]** to return Edit interface, Press **[Save]**.
5. Press **[Esc]** to return and the interface appears with the edited PV curve.

- **Userdefined**

You can customize the editing of the PV curve. The steps to edit a custom curve are as follows:

1. Click SAS on the Menu screen to enter the SAS function main interface.
2. Press **[Edit]** and enter to the PV curve file edit interface.

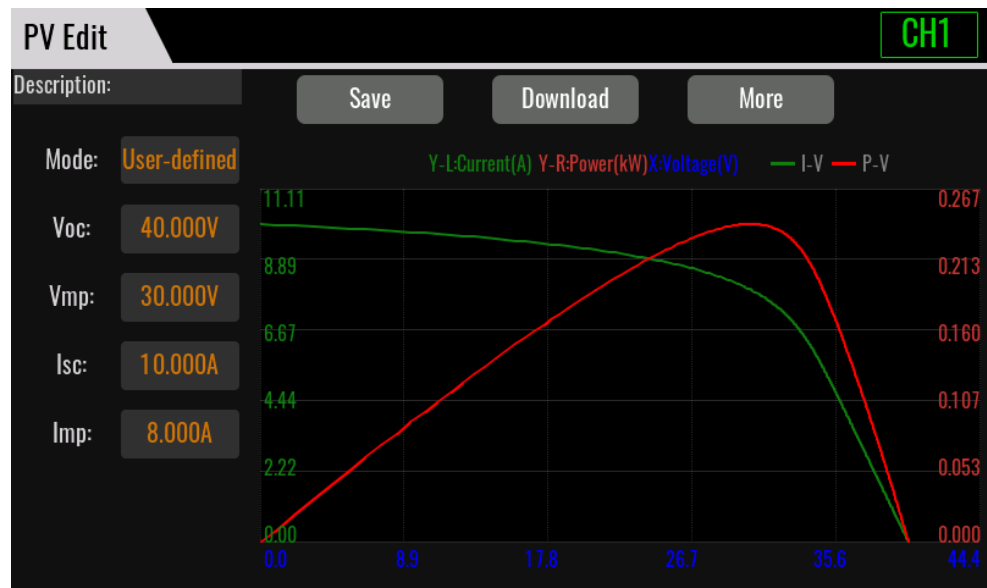

PV edit description:

| Parameter | Description |
|-------------|---|
| Description | Display PV curve file name. |
| Mode | Select the PV curve working mode User-defined or Curve. |
| Voc | Open-circuit voltage value. |
| Vmp | Maximum power voltage value. |
| Isc | Short-circuit current value. |
| Imp | Maximum power current value. |
| Save | Save the PV curve file. |
| Download | Download the SAS configuration to make it effective. |

| Parameter | Description |
|-----------|--|
| More | <ul style="list-style-type: none"> ● Filter: Filter the voltage collected from the output terminals of this instrument to reduce interference factors. Low(Low Speed Filtering), Mid(Medium Speed Filtering), High(High Speed Filtering). ● Priority: Sets the output priority mode, CC or CV. ● Sas Speed: When CC is prioritized, the current loop speed is set; when CV is prioritized, the voltage loop speed is set. |

3. Fill in corresponding parameter in the PV edit interface. Click [More] enter to advanced menu of PV file.
4. Press [**Esc**] to return Edit interface, Press [**Save**].
5. Press [**Esc**] to return and the interface appears with the edited PV curve.

Select/Run PV Curve File

1. Click SAS on the Menu screen to enter the SAS function main interface.
2. Press [**Open**], select the saved PV01 csv file, and press [**Enter**] to enter the file.
3. Press [**Run**] in the SAS function interface will start the MPPT test, and the MPPT efficiency data will be displayed on the PV graph.
4. Running icon will appear in interface.
5. Click [**Stop**] to stop the present running.

Import/Export PV Curve file

- **Import PV Curve file**

IT6600 series support import PV Curve file function, the user can finish the editing of PV Curve file in Excel and import it into the instrument. This function simplifies the PV Curve file edit and facilitates user operation.

To help user define an Excel file format, please export a CSV template from the SAS interface.

Detailed operation steps are as below:

1. Create a new Excel document on local PC and name it 5.csv.
2. Open the Excel document and save it as in "other formats" i.e. "(*.csv)".
3. Open the 5.csv document and edit the PV Curve. Set the parameter values of the PV curve and save the file in the USB disk.

| | A | B | C |
|----|-----------|-------------|---|
| 1 | Model | IT6600 | |
| 2 | File Type | SAS | |
| 3 | Sub Type | Userdefined | |
| 4 | VOC | 40 | |
| 5 | VMP | 30 | |
| 6 | ISC | 10 | |
| 7 | IMP | 8 | |
| 8 | Filter | Low | |
| 9 | Priority | CV | |
| 10 | | | |

4. Insert the USB disk into the USB interface of the front panel.
5. Click SAS on the Menu screen to enter the SAS function main interface.
6. Click the **[Open]** key on the screen, enter to SAS recall interface.
7. Click usb, select the 5.csv file in the usb, and click **[Open]** to confirm. The PV Curve file will be imported and the configured 5.csv file will appear in the interface.

- **Export PV Curve file**

After editing the PV Curve file, the user can directly save it into the device or export and save it into the peripheral memory disc. The exported PV Curve file is saved in the format of. (*.csv). Detailed operation steps are as below:

1. Insert the U disk into the USB interface of the front panel. (The USB type needs to be set as Host.)
2. Click SAS on the Menu screen to enter the SAS function main interface.
3. Click the **[Edit]** key on the screen, enter to PV Curve file edit interface.
4. Click the **[Save]** key to enter the SAS save interface.
5. Click usb, set the FileName of the exported file, and click **[Save]** to confirm the export. Then you can export the PV Curve file from Edit interface to USB disk.

Chapter5 System-Related Functions

5.1 System Menu Reference

Press **[Shift] + [P-set]** (System) to enter the menu function. At this time, LCD displays optional menus. Select and edit the menu items by pressing the Up, Down, Left and Right keys. Specific menu items are shown below. The menu items are shown below.

Source menu

| | | | | |
|--------|--------------------|--------------------------------------|---|--|
| Source | Output Mode | Set the output mode. | | |
| | | Mode | <ul style="list-style-type: none"> ● Series: Configure the instrument to 2-channel series mode. ● Parallel: Configure the instrument to 2-channel parallel mode. ● Dual: Configure the instrument to 2-channel independent output mode. When the output mode of the instrument is configured Dual, the synchronization parameters of both channels can be further configured. | |
| | | Sync | <ul style="list-style-type: none"> ● On: Turns on the 2-channel synchronization mode. ● Off: Turns off synchronization mode. | |
| | | Sync Mode | Synchronization mode. | |
| | | | Track: Set 2-channel to output on/off synchronization and voltage proportional changing. <ul style="list-style-type: none"> ● Reference: Set the voltage proportional relationship among 2-channel. | |
| | | | Onoff Only: Set 2-channel to output on/off synchronization. Duplicate: Set the parameters of 2-channel to be fully synchronized. | |
| | | Remote sense | Set the sense function state. | |
| | | | Status | <ul style="list-style-type: none"> ● On: Enable the remote sense Measurement. ● Off: Disable the sense function. |
| | | Output Rzero | Used to control whether the voltage is quickly zeroed after the output is turned off. | |
| | | | Status | <ul style="list-style-type: none"> ● On: Yes ● Off: No |
| | | External Program | External analog function.(External analog interface is optional.) For detailed introduction of menus and functions, see 5.10 Analogue Function . | |
| | | Measure | Set the measurement speed. | |
| | | | Low | Low mode, measuring every 200ms. |
| | | | Medium | Medium mode, measuring every 100ms. |
| | | | Fast | Fast mode, measuring every 20ms. |
| | Power Unit Setting | Set the power unit: W or kW. | | |
| | Redundant Setting | Set the redundant status: On or Off. | | |

General menu

| | | | |
|---------------|----------------------------|---|---|
| General | Buzzer | Set the buzzer sound. | |
| | | Key Sound | Buzzer on/off for key. |
| | | Warning Sound | Buzzer on/off for warn. |
| | | Protection Sound | Buzzer on/off for protect. |
| | Brightness | Set the screen brightness. | |
| | | 1-10 | Set the screen brightness level. |
| | Factory Default Settings | Select whether to reset the factory default settings or not. | |
| | | Restore | Confirm to reset operation |
| | Power-on Setup | Set the power-on state. | |
| | | Reset | When the instrument is powered on, the instrument will initialize some settings and [On/Off] state. |
| | | Last | When the instrument is powered on, the instrument will remain the same settings and [On/Off] state as last time you turned off the instrument. |
| | | Last-off | When the instrument is powered on, the instrument will remain the same settings as last time you turned off the instrument, but the [On/Off] is Off state. |
| | Parallel Settings | Set the instruments to parallel operation mode. | |
| | | Role | <ul style="list-style-type: none"> ● Single: Set the instrument to single mode, i.e., disable the parallel operation mode. ● Master: Set the instrument to master mode. ● Slave: Set the instrument to slave mode. |
| | | Number | Number of parallel instruments. |
| | Touch Function | Lock the touch screen function. | |
| | | Status | Set the On/Off state. |
| | Knob Immediately Effective | Knob setting will take effect immediately. When set to On, the output value will immediately take effect upon rotating the knob. When set to Off, after adjusting the knob, the output value will only take effect after pressing the Enter key to confirm. | |
| | Language | Set the language of display. | |
| | | English | English |
| | | Chinese | Chinese |
| | Soft Keyboard | Set the soft keyboard | |
| | | On | Turn on the soft keyboard. The soft keyboard will pop up when the edit box is in editing mode. |
| | | Off | Turn off the soft keyboard. |
| | Hover Button | | |
| | | On | Use the hover button for full touch mode operation. |
| | | Off | Turn off the hover button. |
| Communication | USB type | Set the USB type. | |
| | | Device: the USB device is used to communication with PC. | |
| | | Host: the USB device is used to storage disk. | |

| | | | |
|--|------------------|--|---|
| | USB device class | USB communication interface | |
| | | VCP | Virtual serial port |
| | | TMC usbtmc | USB-TMC protocol |
| | LAN Settings | LAN communication interface | |
| | | Mode | <ul style="list-style-type: none"> ● DHCP: automatically configure the address of the instrument. ● Manual: manually configure the address of the instrument by entering values in the following five fields. |
| | | IP | Set the IP address. |
| | | Mask | Set the subnet mask. |
| | | Gateway | Set the gateway address. |
| | | Port | Set the port number. |
| | RS232 Settings | Select RS232 communication interface. When insert IT-E177 communication board into expansion slot, the menu displays this information. | |
| | | Baud rate | Baud rate |
| | | Data bits | Data bit: 5/6/7/8 |
| | | Stop bits | Stop bit: 1/2 |
| | | Even-odd check | Parity bit: N (No parity) / E (Even parity) / O (Odd parity) |
| | | Address | Address |
| | GPIB Settings | Select GPIB communication interface. When insert IT-E176 communication board into expansion slot, the menu displays this information. | |
| | | Address | Set the communication address |
| | CAN Settings | CAN communication interface. | |
| | | Baud rate | Select the baud rate |
| | | Address | Set the instrument address to a number |
| | | Protocol | <ul style="list-style-type: none"> ● CAN_OPEN: High-level protocol for the CAN bus. ● CAN2.0: ITECH CAN version 2.0 protocol. |

IO menu

| | | |
|---------------|--------------------------------------|---|
| IO | Digital IO-1 Settings | Set Digital I/O. For detailed introduction of menus and functions, see 5.9 Digital I/O Function . |
| | Digital IO-2 Settings | |
| | Digital IO-3 Settings | |
| | Digital IO-4 Settings | |
| | Digital IO-5 Settings | |
| | Digital IO-6 Settings | |
| | Digital IO-7 Settings | |
| Information | Product model | Display the instrument model. |
| | SN | Display the serial number. |
| | Software version | Display the system version information. |
| | MAC address | MAC address |
| | Rbf version | Rbf version |
| | Ctrl1 version | Ctrl1 version |
| | Ctrl2 version | Ctrl2 version |
| | Inner numbers | Number of inner ring parallel instruments. |
| Power On Time | The power on time of the instrument. | |

| | | |
|--|---------------------|--|
| | Current Output Time | The current output time of the instrument. |
| | History Output Time | The history output time of the instrument. |

Set the buzzer sound

- **Key Sound:** This item can set the key sound state. If in ON mode, then when you press a button, the power supply will beep. If in OFF mode, the beeper will not make a sound. The default set is in ON mode.
- **Protection Sound:** This item allows you to set the protection sound status. If it is in ON mode, the power supply will beep when protection occurs. If it is in OFF mode, the buzzer will not sound. The default setting is ON mode.
- **Warning Sound:** This item allows you to set the warn sound status. If it is in ON mode, the power supply will beep when a warning occurs. If it is in OFF mode, the buzzer will not sound. The default setting is ON mode.

Set the screen brightness

This item can set the screen brightness. Set the screen brightness within the range 1 to 10 by pressing number keys on the front panel. The larger the number is, the higher the screen brightness is. You can also set the screen brightness by rotating the knob on the front panel. Default setting is 5.

Restored to Factory Setting

This menu item is used to restore all settings of the instrument to factory default values.

The procedures to set the menu item are as follows.

1. Select the **General** under system menu.
2. Press **Restore** in Factory Default Settings.

Set the Power-on State

This parameter determines the state of the DC source after power up.

The procedures to set the menu item are as follows.

1. Press the **General** under the system menu.
2. Press the Up/Down key or turn the knob to select the **Power-on setup** and press **[Enter]**.
 - **Reset:** Default value, indicates when the instrument is powered on, the instrument will initialize some parameter settings or state, such as output voltage, output current and output status.
 - **Last:** Indicates when powered on, the instrument will remain the same parameter settings and output status as last time you powered off the instrument.
 - **Last+Off:** Indicates when powered on, the instrument will remain the same settings as last time you powered off the instrument, but the output status is **Off**.

Set the Knob Function

Set the knob setting function. If set to ON, the Knob setting will take effect immediately. If set to OFF, press Enter to confirm the effect after the Knob setting is completed.

Select Language

Users can select the instrument language type from the menu.

Set the Soft Keyboard

The user can open the soft keyboard in the menu. When the parameter is set to ON, the soft keyboard is enabled. And when setting parameters on the screen, the soft keyboard appears. Convenient users directly touch screen to select the number.

5.2 Configuration Menu Reference


Press **[Shift] + [V-set]** (Config) key and enter to configuration menu interface. At this interface, user can setup the power supply output parameters, detailed parameters are shown as follows.

| Config | Configuration menu of the power supply. | | |
|--------------------|---|---|---|
| | Priority Mode | CC/CV priority mode setting. | |
| | | Mode | Mode Settings. |
| | | | CV: Constant voltage loop priority mode. |
| | | | CC: Constant current loop priority mode. |
| | | Loop Speed | Loop response speed setting. |
| | | | High: high speed. |
| | | | Medium: medium speed. |
| | | Low: low speed. | |
| | | Only Load | Load mode only. (This item is only displayed when CC is prioritized.) |
| | | Battery Simulation | Battery simulator mode. (This item is only displayed when Only Load is enabled.) |
| | Slew Config | Slew Setting. | |
| | | Mode | Select the slew unit. |
| | | | Time: describe the slew of the device in terms of time. |
| | | | Standard: standard slew, unit is V/ms or A/ms. |
| | | V-Rise/ I-Rise | Displays the voltage or current rise slew setting according to the selected priority mode. If CC priority mode is selected, the parameter setting of I-Rise will be displayed here. |
| | V-Fall/ I-Fall | Displays the voltage or current fall slew setting according to the selected priority mode. If CC priority mode is selected, the parameter setting of I-Fall will be displayed here. | |
| Output Couple Mode | Set the output mode. | | |
| | Mode | | |
| | | DC: DC mode. | |
| Output Resistance | Set the internal resistance of the power supply. (This item is only displayed when CV is prioritized.) | | |
| Onoff Delay | | | |
| | On Delay | Set the delay time to turn on the output. | |
| | | Offset : Set the output delay offset time. | |

| | | | |
|--|--|-----------|--|
| | | Off Delay | Set the delay time to turn off the output. |
|--|--|-----------|--|

5.3 Key Lock Function

Press **[Shift] + [2]** (Lock) button to set the key lock state. If keyboard has been

locked, the indicator light  will display on the LCD. In addition, when keyboard are locked, all buttons can't be used except Local key Press **[Shift] + [2]** (Lock) once again will relieve key lock function.

5.4 Switching Local/Remote Mode

You can press the **[Shift] + [3]** (Local) button to change the DC source from remote to local operation.

After you power on the DC source, it defaults in local mode, all buttons are enabled. While in remote mode, most buttons are disabled except **[Shift] + [3]** (Local) keys. You can switch Local/Remote mode via PC. In addition, the mode modification will not affect the output parameters.

5.5 Save and Recall Operations

The power system can save up to 100 common parameters in nonvolatile memory (No. 1 to No. 100) for user to recall conveniently.


The saved parameters include:

- Power supply mode
- Present output parameters
- Config menu settings

Save Operation

The save operation procedures are as follows:

1. Press the composite keys **[Shift]+[4]**(Save) to enter the parameter save interface.
2. Select the storage location. up to 100 position can be select.

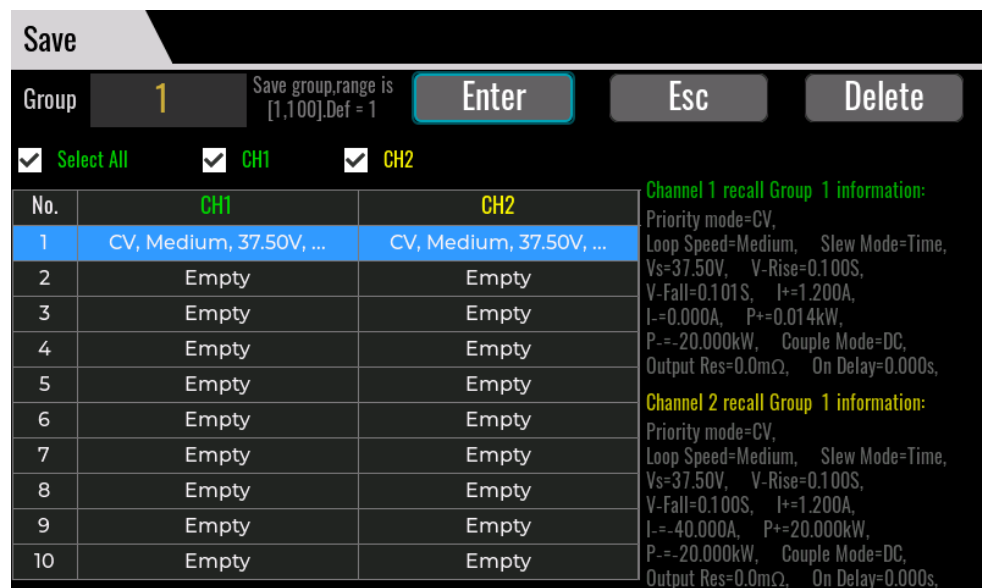

Save

Group **1** Save group range is [1,100].Def = 1

Select All CH1 CH2

| No. | CH1 | CH2 |
|-----|-------------------------|-------------------------|
| 1 | CV, Medium, 37.50V, ... | CV, Medium, 37.50V, ... |
| 2 | Empty | Empty |
| 3 | Empty | Empty |
| 4 | Empty | Empty |
| 5 | Empty | Empty |
| 6 | Empty | Empty |
| 7 | Empty | Empty |
| 8 | Empty | Empty |
| 9 | Empty | Empty |
| 10 | Empty | Empty |

Channel 1 recall Group 1 information:
 Priority mode=CV,
 Loop Speed=Medium, Slew Mode=Time,
 Vs=37.50V, V-Rise=0.100S,
 V-Fall=0.101S, I+=1.200A,
 I-=0.000A, P+=0.014kW,
 P-=20.000kW, Couple Mode=DC,
 Output Res=0.0mΩ, On Delay=0.000s,

Channel 2 recall Group 1 information:
 Priority mode=CV,
 Loop Speed=Medium, Slew Mode=Time,
 Vs=37.50V, V-Rise=0.100S,
 V-Fall=0.100S, I+=1.200A,
 I-=40.000A, P+=20.000kW,
 P-=20.000kW, Couple Mode=DC,
 Output Res=0.0mΩ, On Delay=0.000s,

3. Press **[Enter]** to save the parameters.

Finished, the saved parameters will be display at the right side of the interface.

Recall Operation

You can recall the parameters you saved in the specified memory location as the setting values.

1. Press the **[Recall]** key to enter the parameter recall interface.
2. Set the storage location.

Press the direction keys to set the storage location, and then, the saved parameters will be display at the bottom of the interface.



The screenshot shows the 'recall' interface with the following components:

- Group:** 1 (Recall group, range is [1,100], Def = 1)
- Buttons:** Enter, Esc, Delete
- Checkboxes:** Select All, CH1, CH2 (all checked)
- Table:**

| No. | CH1 | CH2 |
|-----|-------------------------|-------------------------|
| 1 | CV, Medium, 42.49V, ... | CV, Medium, 37.50V, ... |
| 2 | Empty | Empty |
| 3 | Empty | Empty |
| 4 | Empty | Empty |
| 5 | Empty | Empty |
| 6 | Empty | Empty |
| 7 | Empty | Empty |
| 8 | Empty | Empty |
| 9 | Empty | Empty |
| 10 | Empty | Empty |
- Channel 1 recall Group 1 information:**
 - Priority mode=CV, Loop Speed=Medium, Slew Mode=Standard, Vs=42.49V, V-Rise=50.000V/ms, V-Fall=50.000V/ms, I+=1.200A, I-=0.000A, P+=0.014kW, P-=-20.000kW, Couple Mode=DC, Output Res=0.0mΩ, On Delay=0.000s,
- Channel 2 recall Group 1 information:**
 - Priority mode=CV, Loop Speed=Medium, Slew Mode=Time, Vs=37.50V, V-Rise=0.100S, V-Fall=0.100S, I+=1.200A, I-=40.000A, P+=20.000kW, P-=-20.000kW, Couple Mode=DC, Output Res=0.0mΩ, On Delay=0.000s,

3. Press **[Enter]** to recall the parameters.

5.6 Screen Capture Function

IT6600 series power supply has the screen capture function. Insert the USB equipment into the USB interface of the front panel, and press **[Print]** on the front panel to capture and save the current screen into the USB disk.

When you need the screen capture function, the USB type under the system menu needs to be set to **Host**.

5.7 Query the System Log

The IT6600 series power supply provides the system operation Log query function. On the Menu interface of the front panel of the instrument, click Log or directly press **[Shift]+[1]**(Log) to enter the Log query interface. You can view historical system operation records on this screen.


5.8 Multi-units operation

5.8.1 Series Operation(single-unit)


The IT6600 power supply can increase its output voltage and power by connecting the two channels of a single instrument in series. When connected in series, the upper limit of the voltage setting range is twice the rated value of a single channel, and the instrument is used as a single channel power supply at this time.

Operation steps

1. Set the two channels of the power supply to **Series** mode.
 - a) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - b) Select the **Source** tab, then press the up/down key or rotate the knob to find **Output Mode** menu.
 - c) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to set **Series** output mode, and press the **[Enter]** key to confirm.
2. Refer to the figure below to connect the DUT, and live wiring is prohibited.
 - Local sense

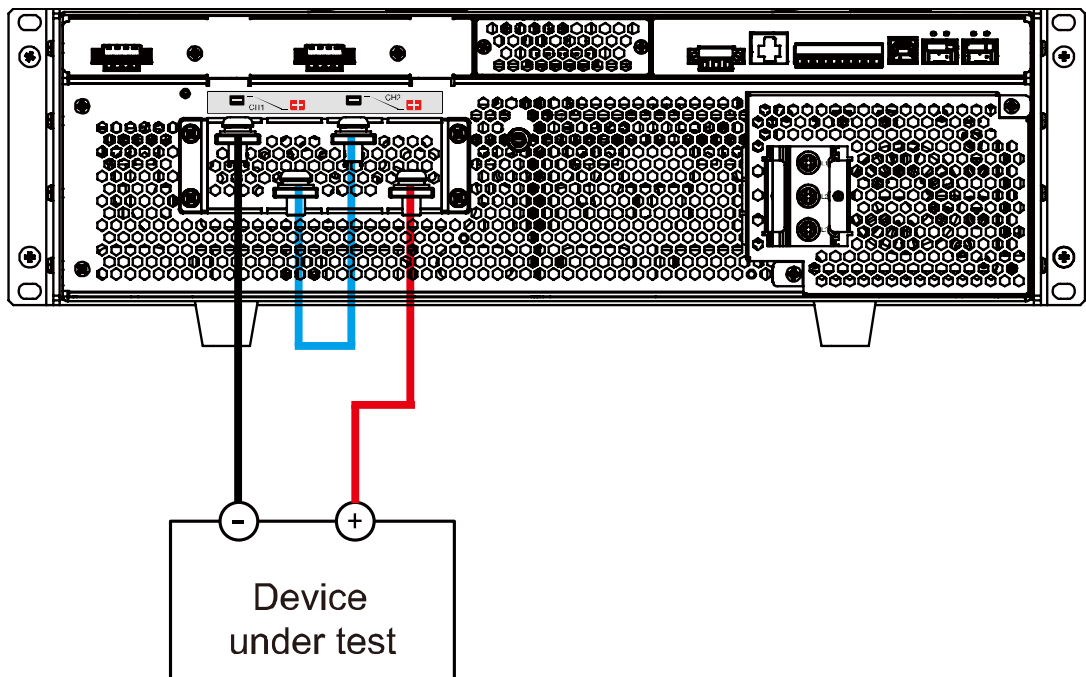

- Remote sense

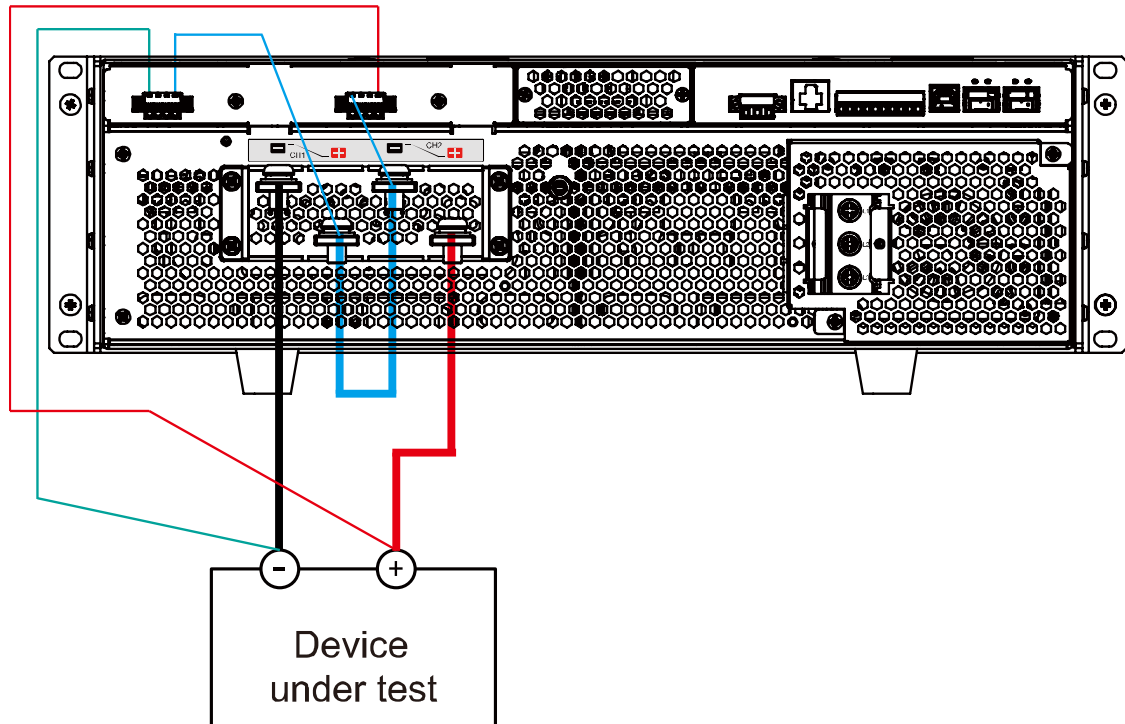


5.8.2 Parallel Operation(single-unit)


The IT6600 power supply can increase its output current and power by connecting the two channels of a single instrument in parallel. When connected in parallel, the upper limit of the current setting range is twice the rated value of a single channel, and the instrument is used as a single channel power supply at this time.

Operation steps

1. Set the two channels of the power supply to **parallel** mode.
 - a) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - b) Select the **Source** tab, then press the up/down key or rotate the knob to find **Output Mode** menu.
 - c) Press the up/down key to move the cursor to the **Mode** function setting and press the **[Enter]** key to confirm. Rotate the knob to set **Parallel** output mode, and press the **[Enter]** key to confirm.
2. Refer to the figure below to connect the DUT, and live wiring is prohibited.
 - Local sense

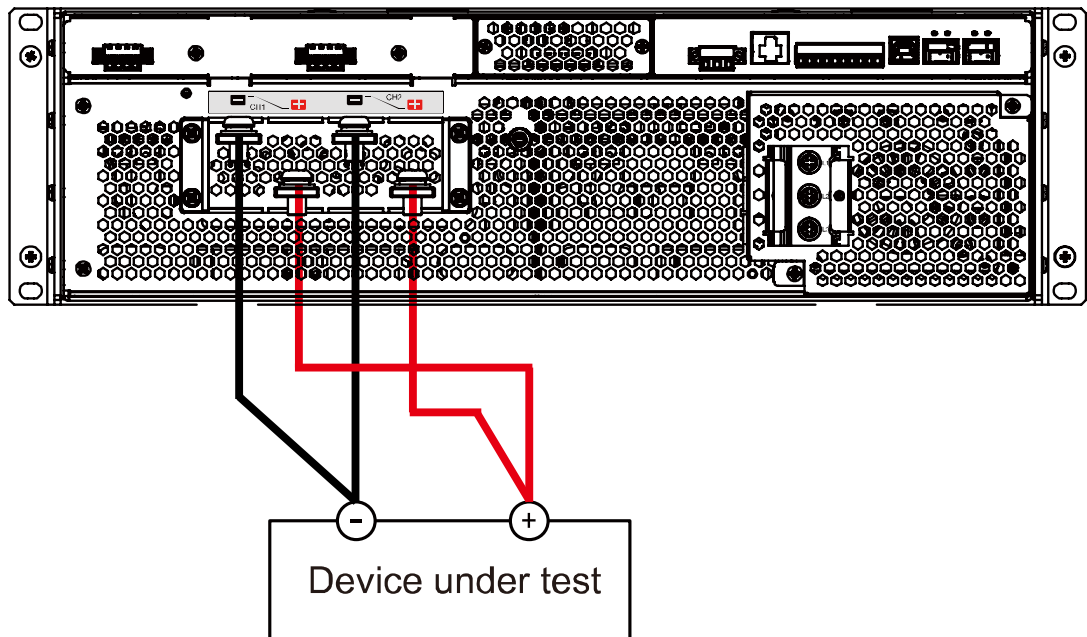

- Remote sense

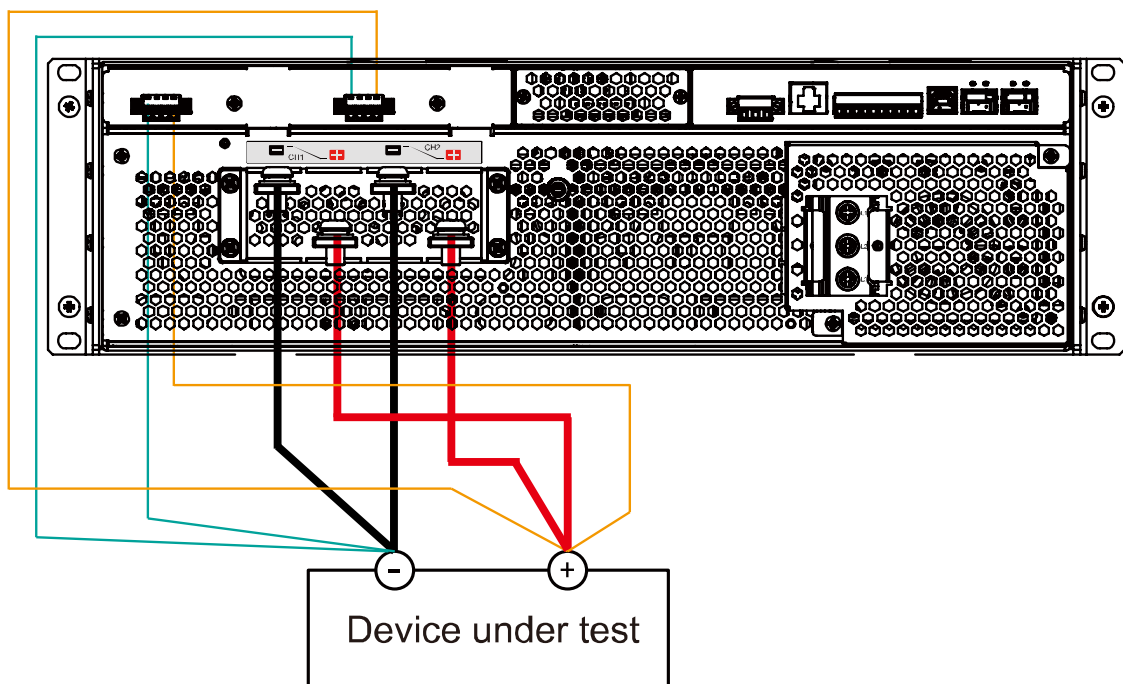

5.8.3 Parallel Operation(multi-masters)

The IT6600 series power supply supports multiple instruments to work in parallel mode to provide more power and current output capability. Under the parallel mode, all features are set up from the master unit.


This chapter takes three instruments (with operation panel) as an example to describe how to parallelize the single units and how to return from parallel mode to single mode.

Set the Parallel Mode


WARNING

- Before connecting the cables, ensure that the instrument power switch is off and the main switch of the AC power input (distribution box) is off.
- Before connecting 3 single instruments to the AC distribution box, ensure that the distribution box capacity is sufficient. Refer to the corresponding specifications for the AC input parameters of a single instrument.
- Before connecting the system bus, you must ensure that each instrument is in single mode (Single).
- Fiber optic cables cannot be flexed or folded. When the cable is too long and needs to be arranged, gently wrap the cable in a circle and gently tie it.

1. Ensure that the power switches of the three units and the main switch of the AC power distribution box are off.
2. Connect the instruments according to the following diagram.
 - In dual-channel mode, the wiring schematic is shown below.

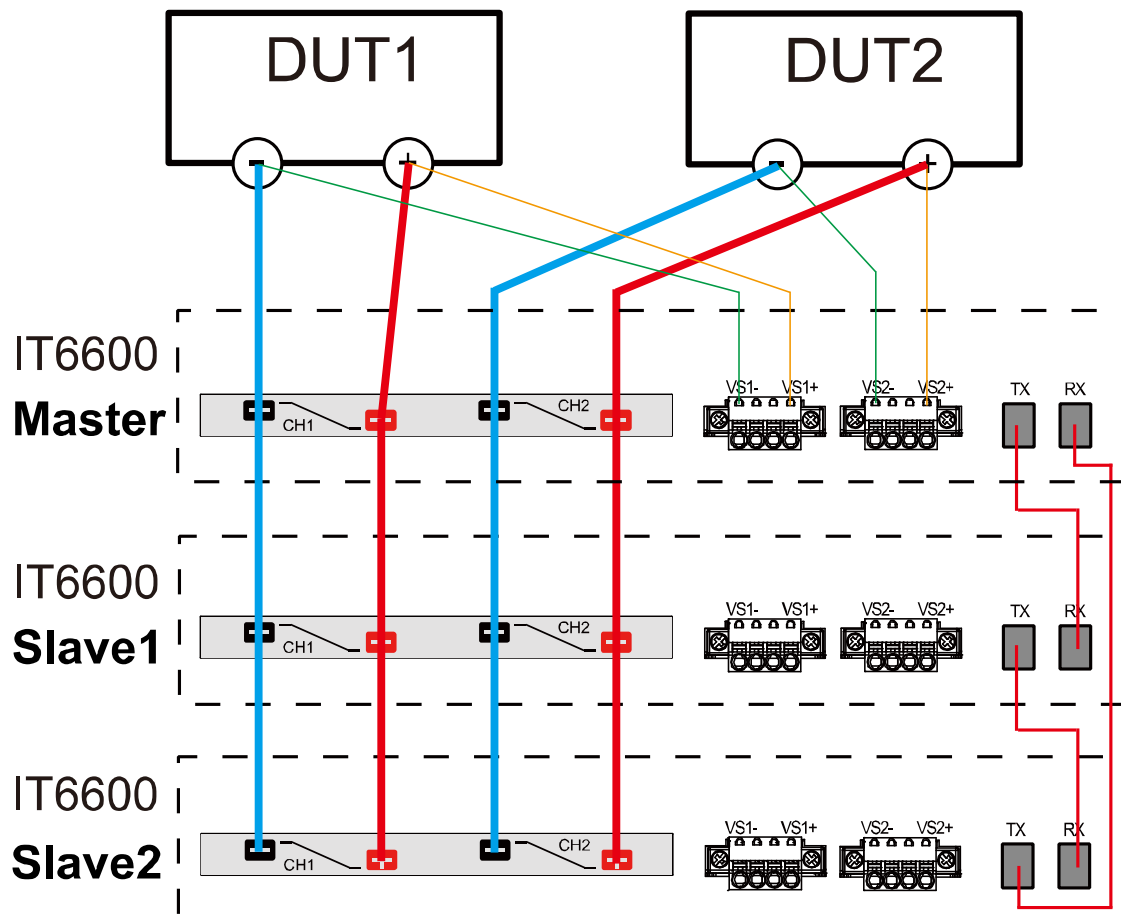


- In series mode, the wiring schematic is shown below.


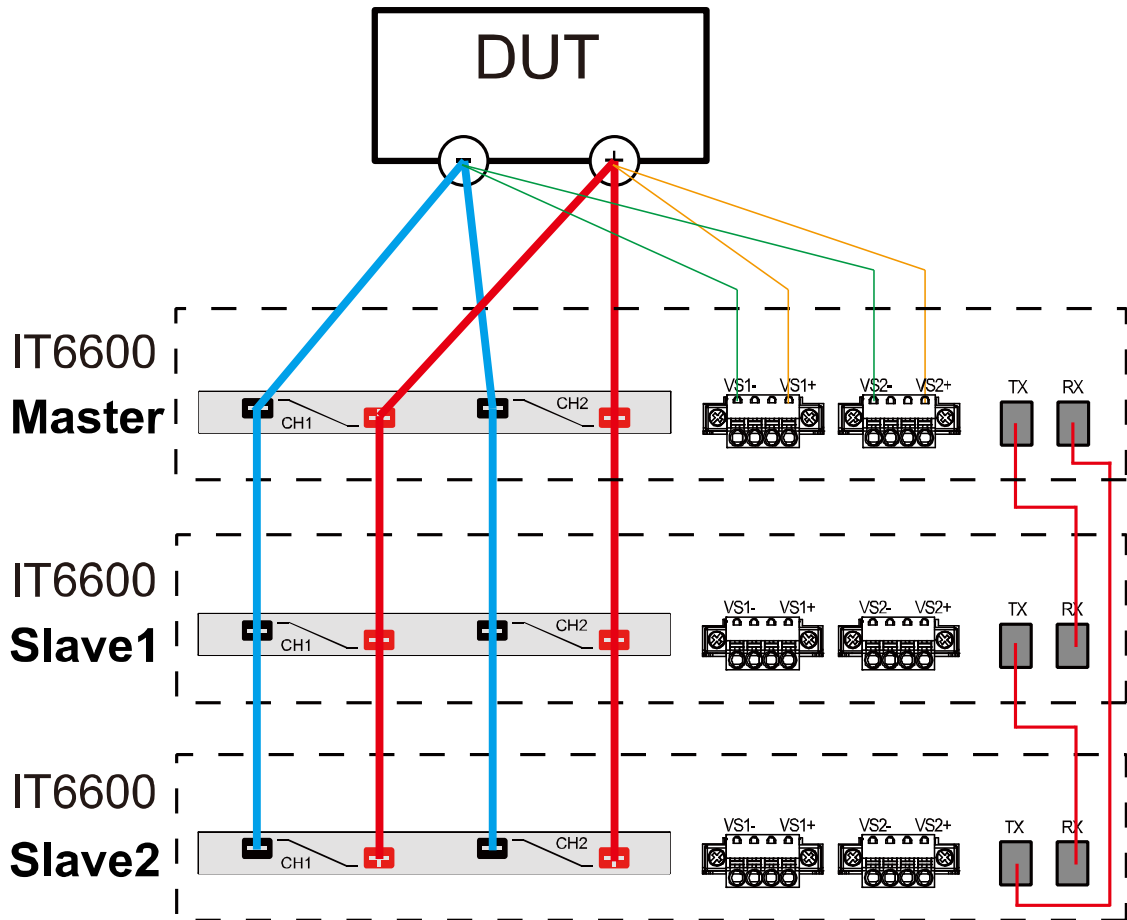


- Connect the DC output terminals of the three instruments in parallel and connect them to the device under test according to different output modes.
- Refer to the blue wiring legend in the figure, connect the System Bus (i.e., the fiber outer ring interfaces TX and RX) for fiber-optic communication between the master and slaves.

Insert the fiber optic module into the hole corresponding to TX RX.

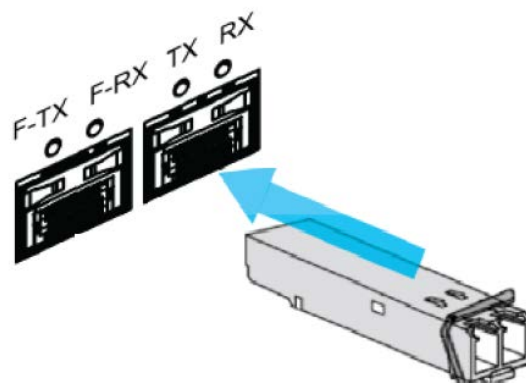

Insert the plug of the fiber optic cable into the fiber optic module and hear a click sound to indicate that it is inserted in place. The fiber optic cable connection schematic is as follows.

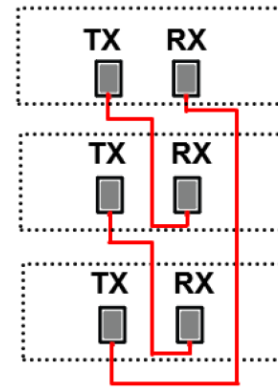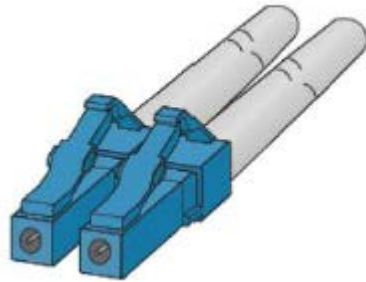

3. After connection, configure one power supply as a master unit and other power supplies as slave units.
 - a) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - b) Press the up/down key or rotate the knob to find **General->Parallel Settings** menu.
 - c) Set the **Role**, set them to one master unit and two slave units. In each group, one instrument must be the master unit and all other instruments connected in parallel are slave units. All features are set up from the master unit.
 - Single: Default value, indicates that the instrument is in single mode.
 - Master: Indicates that the single unit is set to master in parallel mode.
Numbers: total number of units in the parallel relationship, when the instrument set to master, you need to set the Numbers. For example, Numbers set to 3.
 - Slave: Indicates that the instrument is set to the slave in parallel mode.
 - d) Press **[Esc]** to exit.
4. After making the master-slave setting, to ensure normal operation, you need to restart the power supplies.

Revert to single mode

To change Parallel Mode to Single Mode, follow the steps below:

1. Switch three instruments into single mode respectively.
 - a) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - b) Press the up/down key or rotate the knob to find **General->Parallel Settings** menu.
 - c) Set the **Role**, set them to single.
2. Power off the three instruments and turn off the main switch of the AC distribution box.
3. Remove the cables connection of the System Bus and output terminals between three units.
4. Power on the three instruments separately. After the instrument is restarted,

the screen shows that the instrument is working in single mode.

5.8.4 Parallel Operation(one master and multi-slaves)


“One master and multiple slaves” means that there is only one instrument with operating panel (namely, the master) in the parallel system, and the other instruments have no operating panels (namely, the slaves). In the “one master and multiple slaves” system, you only need to operate the master’s front panel.

This section uses three instruments as an example to introduce the steps for parallel connection with one master and two slaves. The type and assembly method for parallel connection of other quantities of instruments are the same.


WARNING

- Before connecting the cables, ensure that the instrument power switch is off and the main switch of the AC power input (distribution box) is off.
- Before connecting 3 single instruments to the AC distribution box, ensure that the distribution box capacity is sufficient. Refer to the corresponding specifications for the AC input parameters of a single instrument.
- Fiber optic cables cannot be flexed or folded. When the cable is too long and needs to be arranged, gently wrap the cable in a circle and gently tie it.


1. Ensure that the power switches of the master unit and the main switch of the AC power distribution box are off.
2. Connect the instruments according to the following diagram.
 - In dual-channel mode, the wiring schematic is shown below.

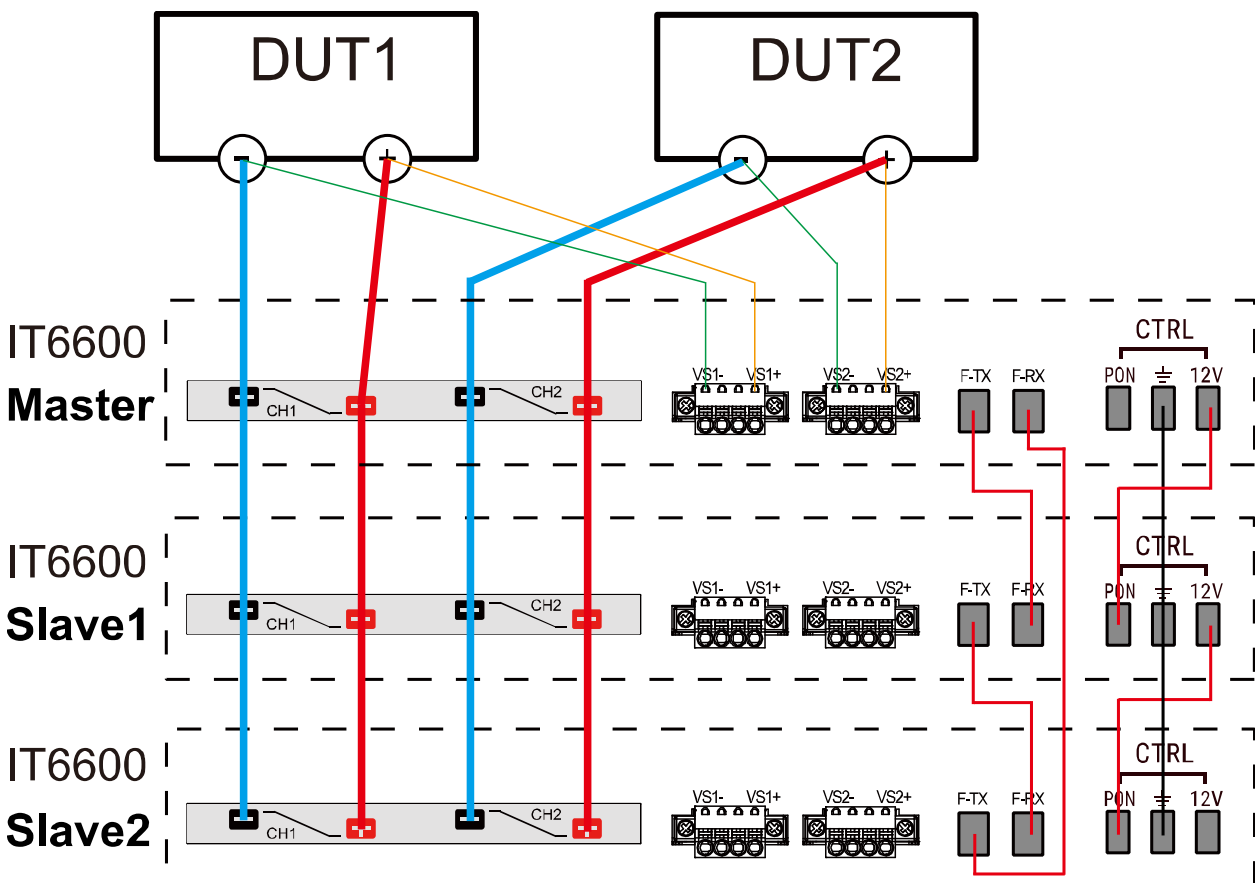

- In series mode, the wiring schematic is shown below.

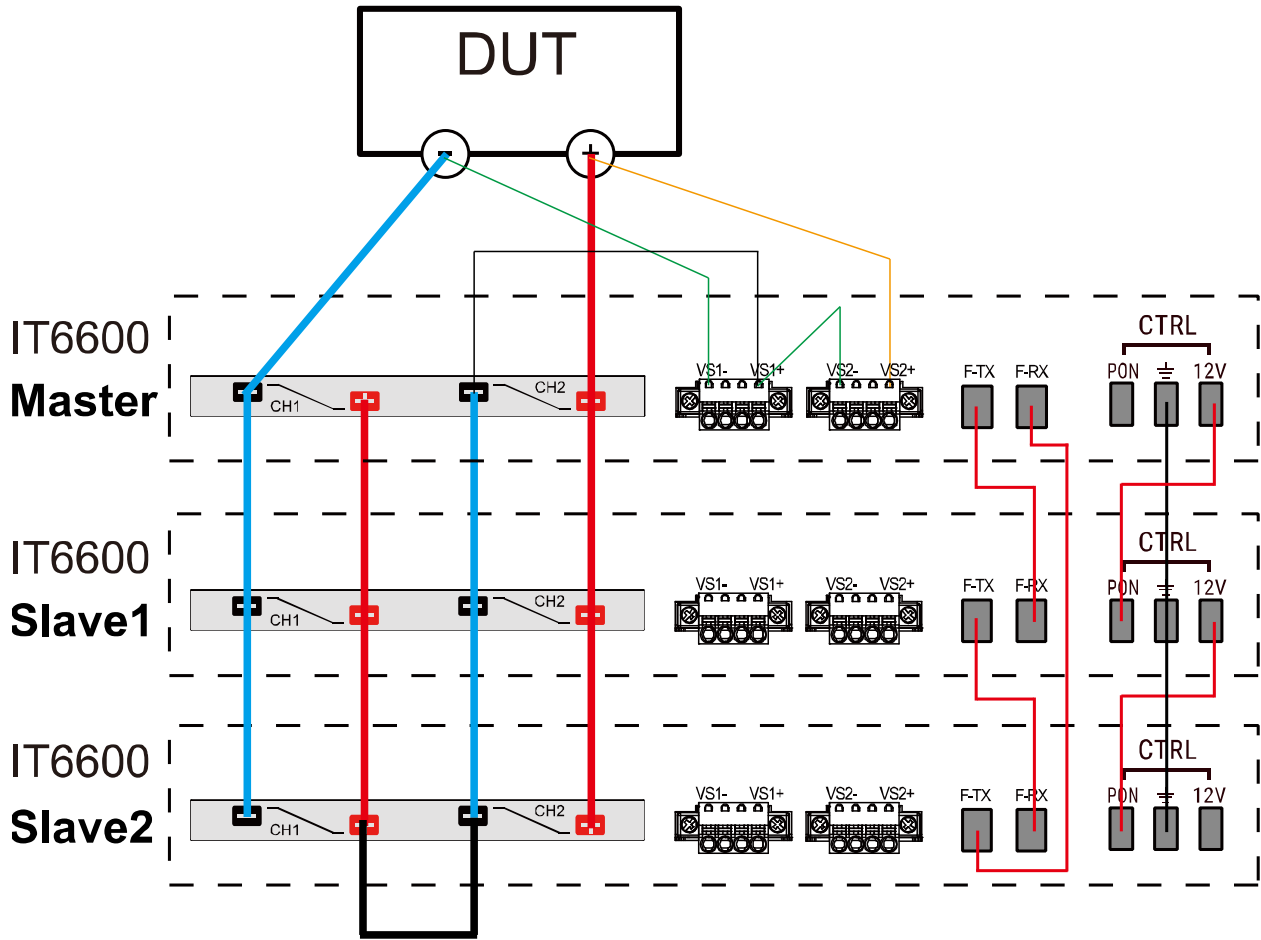

- In parallel mode, the wiring schematic is shown below.

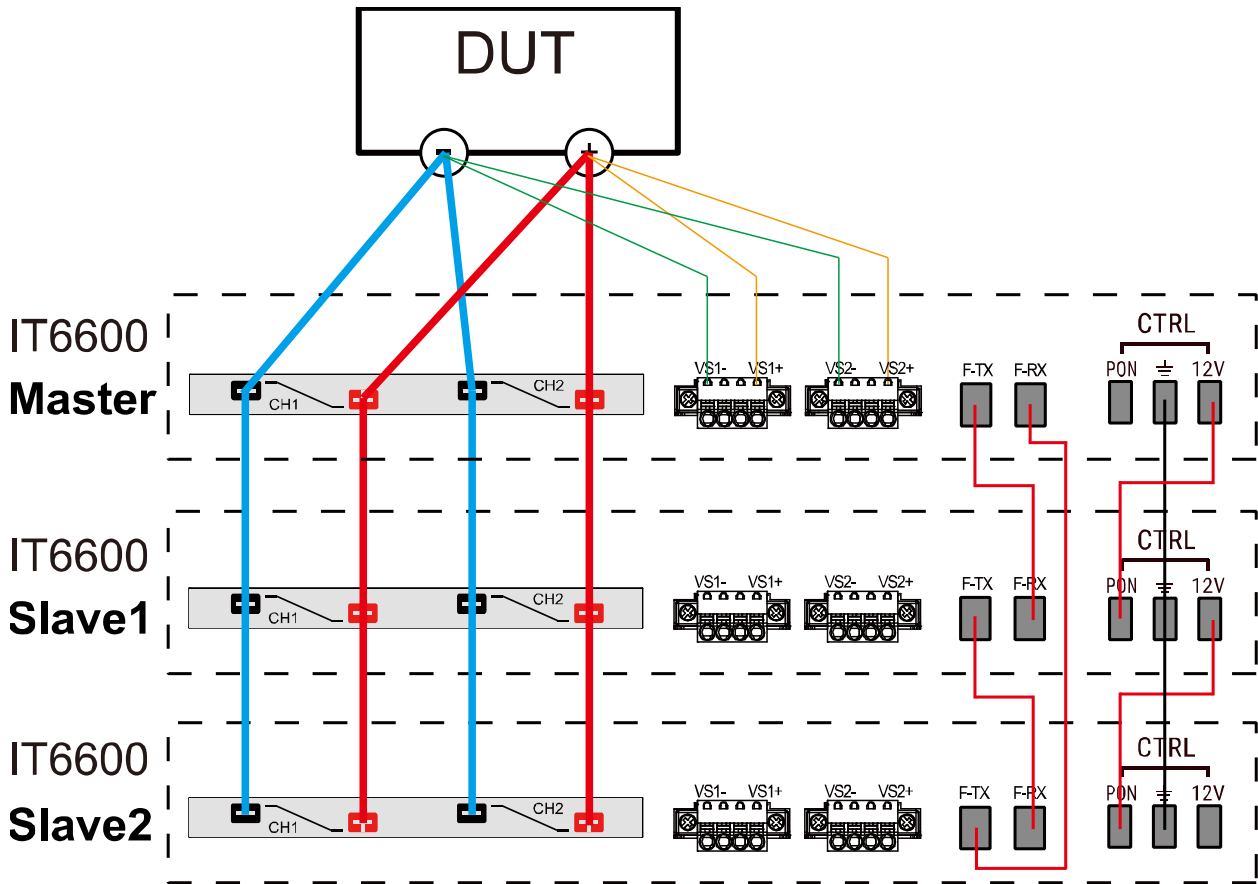


- Connect the DC output terminals of the three instruments in parallel and connect them to the device under test according to different output modes.

- Connect the CTRL cables.

Wiring rules are as follows: Connect the GND/12V of the first single unit to the second single unit's GND/PON, and the second single unit's GND/12V to the third single unit's GND/PON, and so on, until the last single unit is connected.

- Refer to the wiring legend in the figure, connect the System Bus (i.e., the fiber inner ring interfaces F-TX and F-RX) for fiber-optic communication between the master and slaves.

Insert the fiber optic module into the hole corresponding to F-TX, F-RX. Insert the plug of the fiber optic cable into the fiber optic module and hear a click sound to indicate that it is inserted in place.

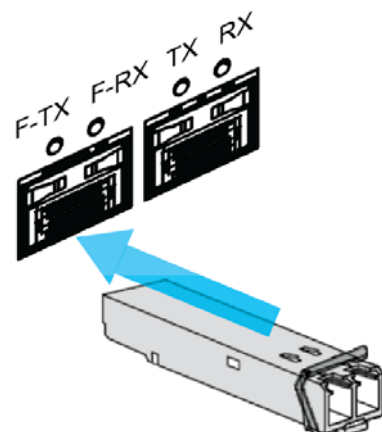

3. Configuring the Master and Slave
 - a) Turn on the power switch on the front panel of the Master unit.
 - b) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - c) Press the up/down key or rotate the knob to find **General->Parallel Settings** menu.
Set the **Role**, set instrument with operating panel to single unit.
 - d) In the Info interface, press the combination key of **[Shift] + [.] + [3] + [8]**.
Set the number of inner ring parallel instruments, such as Inner Number = 3, and press **[Enter]**.
 - e) Turn off the power switch on the front panel of the Master unit. After the power is turned off completely, turn on the power switch again.
4. After the instrument is restarted, the parallel operation is complete.


5.8.5 Parallel Operation(cabinet model)

For cabinet models, the same voltage level can be connected in parallel. Taking two 15U instruments (with operation panel) as an example, the steps for parallel operation are as follows.


WARNING

- **Before connecting the cables, ensure that the instrument power switch is off and the main switch of the AC power input (distribution box) is off.**
- **Before connecting 3 single instruments to the AC distribution box, ensure that the distribution box capacity is sufficient. Refer to the corresponding specifications for the AC input parameters of a single instrument.**
- **Before connecting the system bus, you must ensure that each instrument is in single mode (Single).**
- **Fiber optic cables cannot be flexed or folded. When the cable is too long and needs to be arranged, gently wrap the cable in a circle and gently tie it.**


1. Ensure that the power switches of the two cabinets and the main switch of the AC power distribution box are off.
2. Connect the cabinets according to the following diagram.
 - In dual-channel mode, the wiring schematic is shown below.

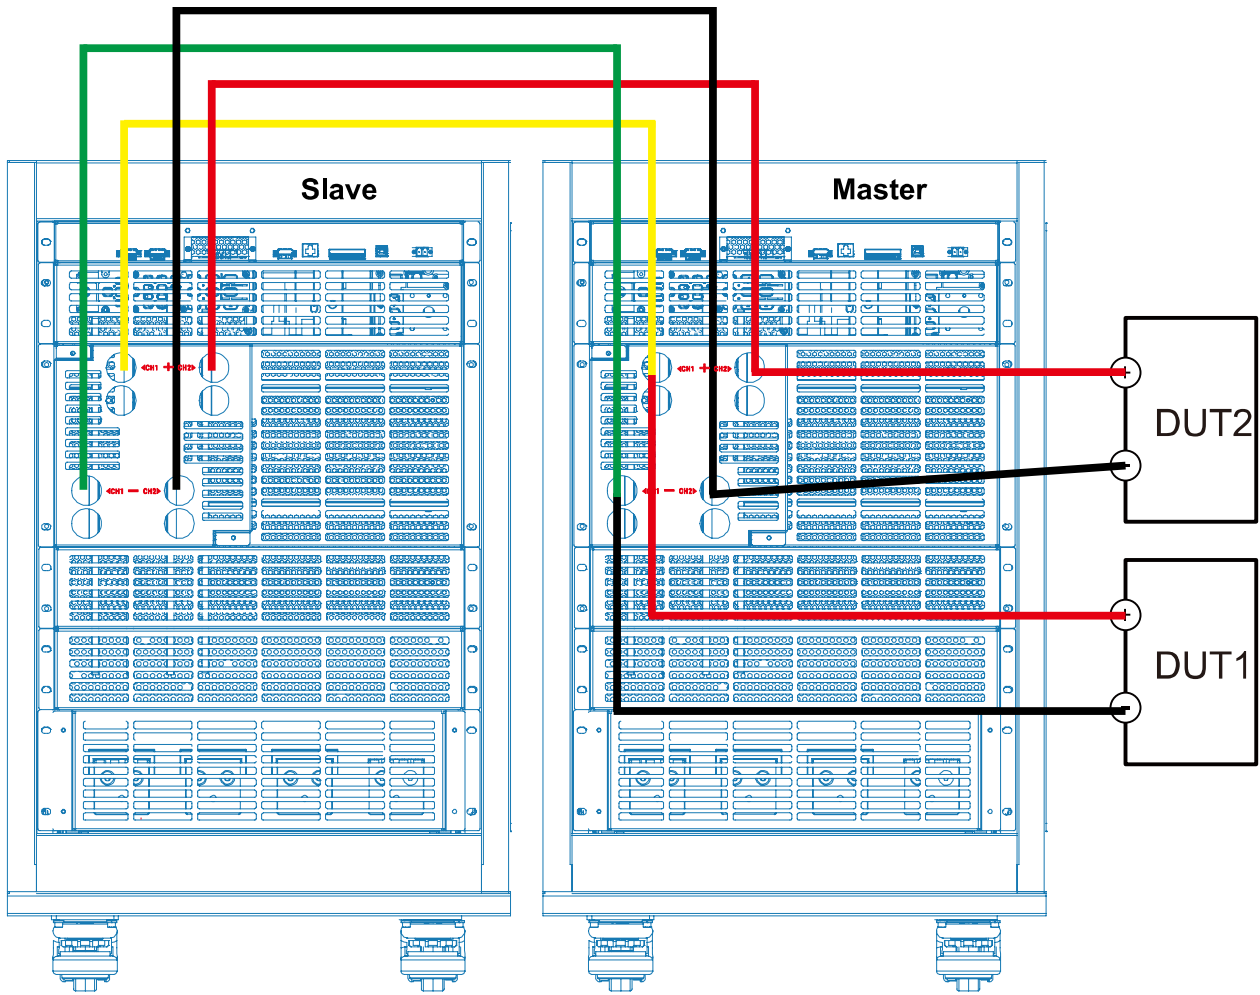

- In series mode, the wiring schematic is shown below.

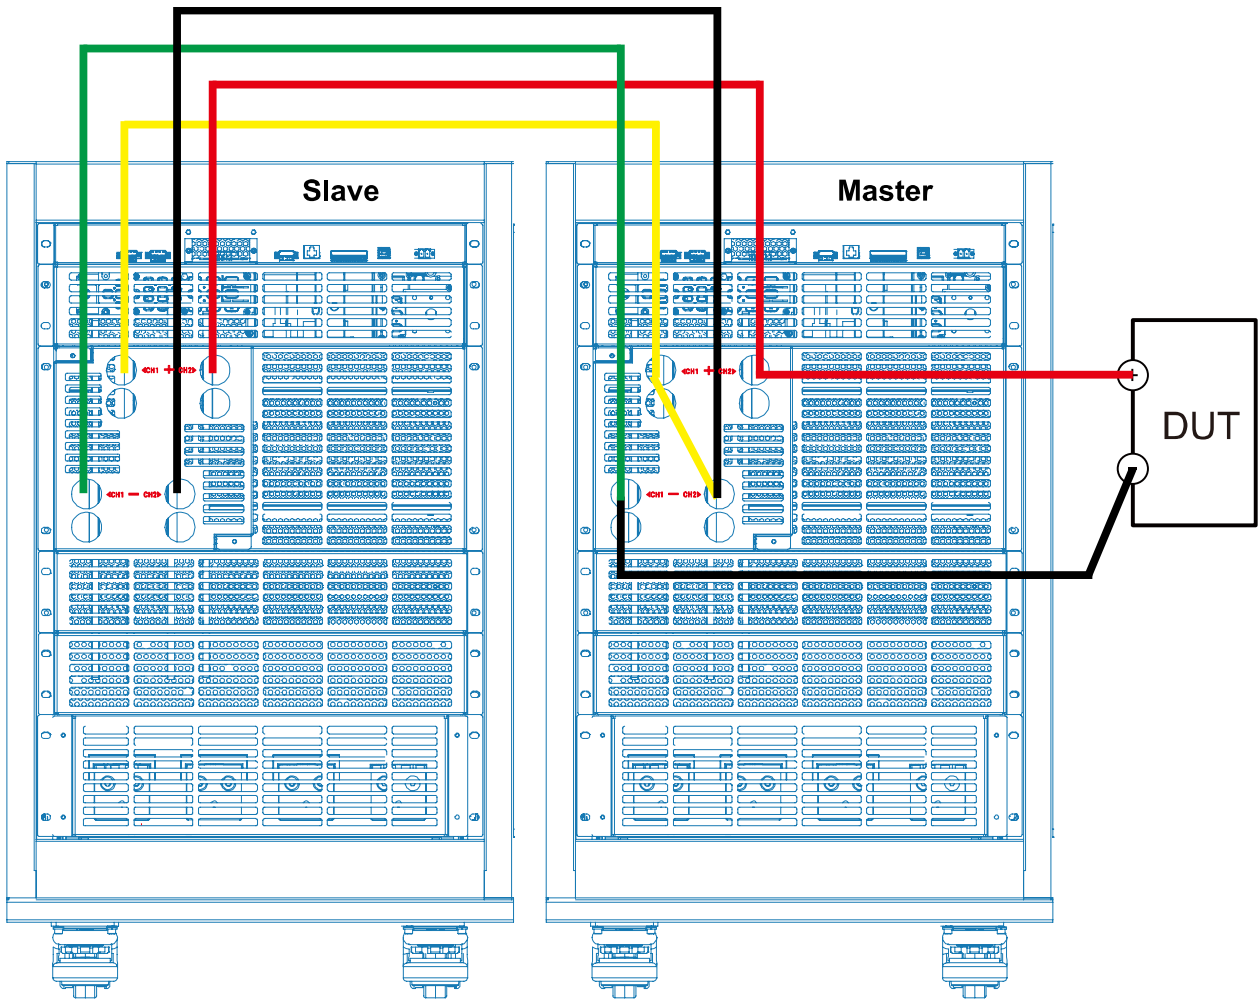


- In parallel mode, the wiring schematic is shown below.


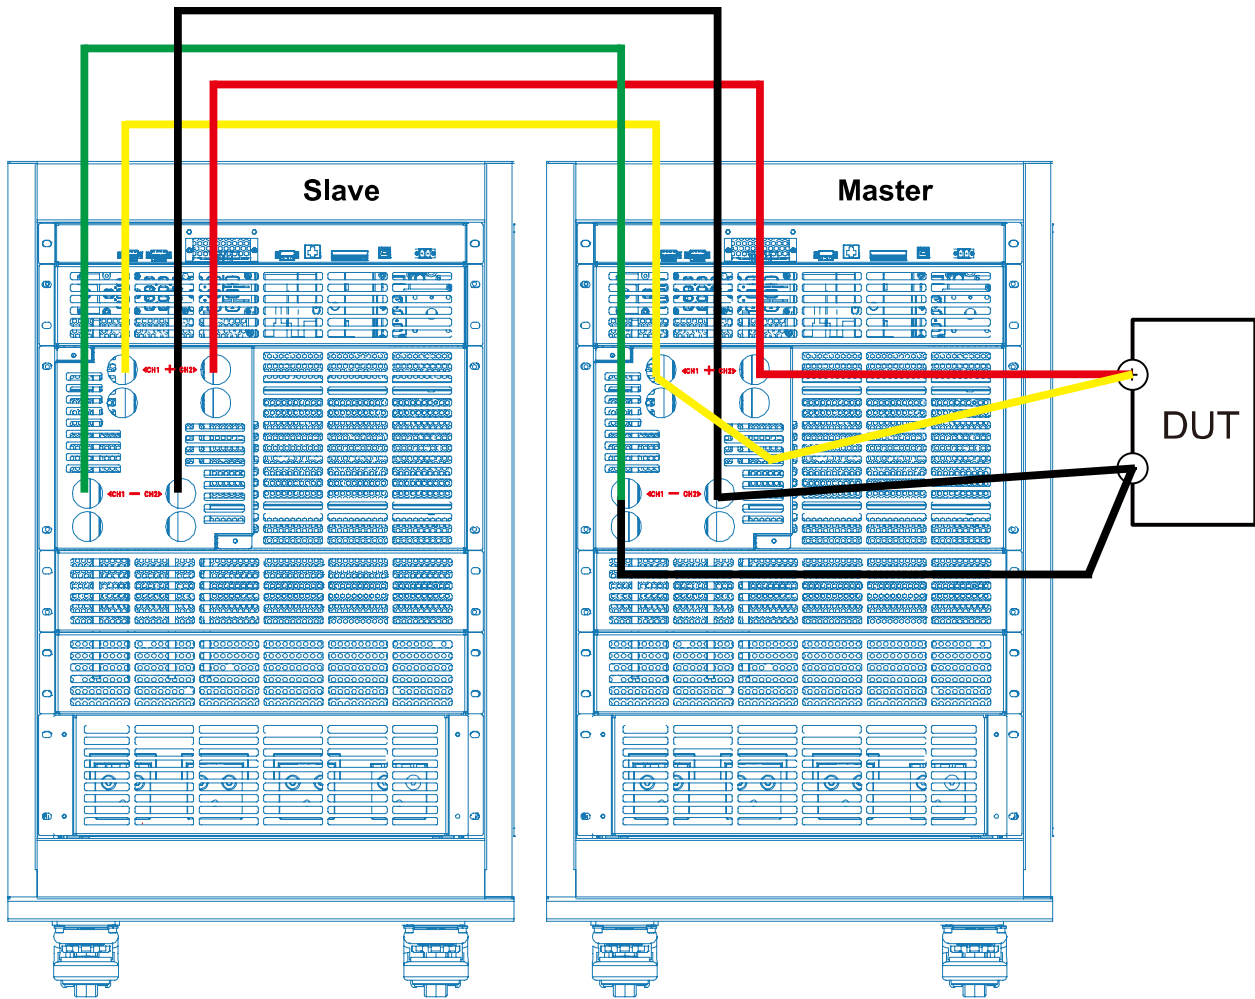


- a) Connect the DC output terminals of the two cabinets in parallel and connect them to the device under test according to different output modes.
- c) Refer to the figure below, connect the System Bus (i.e., the fiber outer ring interfaces TX and RX) for fiber-optic communication between the master and slaves.

Insert the fiber optic module into the hole corresponding to TX RX.

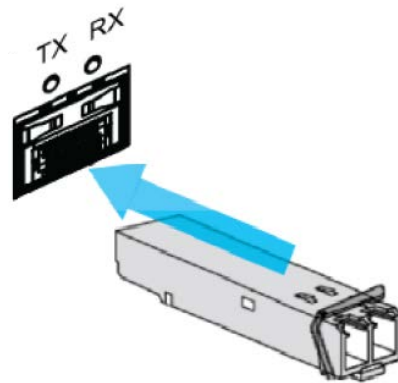


Insert the plug of the fiber optic cable into the fiber optic module and hear a click sound to indicate that it is inserted in place. The fiber optic cable connection schematic is as follows.

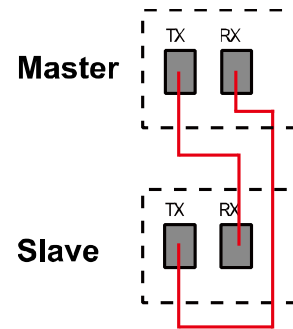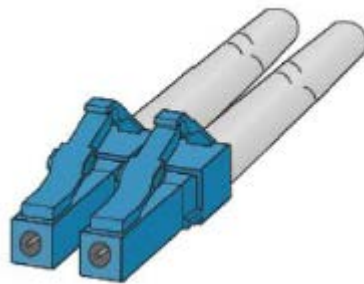

3. After connection, configure one cabinet as a master unit and other cabinets as slave units.
 - a) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - b) Press the up/down key or rotate the knob to find **General->Parallel Settings** menu.
 - c) Set the **Role**, set them to one master unit and one slave unit. In each group, one cabinet must be the master unit and all other cabinets connected in parallel are slave units. All features are set up from the master unit.
 - Single: Default value, indicates that the cabinet is in single mode.
 - Master: Indicates that the single unit is set to master in parallel mode.
Numbers: total number of units in the parallel relationship, when the cabinet set to master, you need to set the Numbers. For example, Numbers set to 2.
 - Slave: Indicates that the cabinet is set to the slave in parallel mode.
 - d) Press **[Esc]** to exit.
4. Turn off the power switch on the front panel of the cabinet in turn. After the power is turned off completely, turn on the power switch again.
After the cabinets are restarted, the parallel operation is complete.

5.9 Digital I/O Function

This series power supply supports digital I/O function. The user can realize logic control over high and low level input or output by related configurations in the system menu. The appearance of the terminals are shown below.

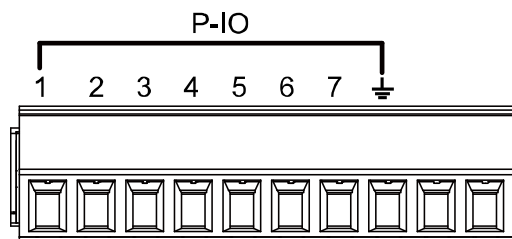

5.9.1 Description of Digital I/O pin

A Digital Control Port consisting of seven I/O pins is provided to access various control functions. Each pin is user-configurable.

Taking pin 3 as an example, IO-3 contains three function options, the first option **Off Status** is the default function, and this function is also a special custom function unique to this pin (the seven pins each have a different custom function). The second and third options (**Input** and **Output**) are the general digital I/O function, and the parameter settings and functions of the seven pins are the same.

Description of Digital I/O pin parameter

Press **[Shift] + [P-set]** (System) to access the system menu functionality page, then select the IO tab to configure relevant parameters.

| | | | |
|----|-----------------------|---|--|
| IO | Digital IO-1 Settings | Function setting of pin 1. | |
| | | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid signal is reversed. |
| | | Function | <ul style="list-style-type: none"> ● PS Clear: This default function means that when the instrument generates protection, the protection state can be cleared via this pin. ● Input: Pin 1 receives the level signal from the outside. ● Output: Pin 1 sends the digital signal (1, 0) to the outside. ● PWM: Pin 1 sends the PWM signal to the outside. |
| | Digital IO-2 Settings | Function setting of pin 2. | |
| | | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid signal is reversed. |
| | | Function | <ul style="list-style-type: none"> ● PS: This default function means the output level from pin 2, which displays that whether the instrument is under protection or not. ● Input: Pin 2 receives the level signal from the outside. ● Output: Pin 2 sends the digital signal (1, 0) to the outside. ● PWM: Pin 2 sends the PWM signal to the outside. |
| | | Channel (Displayed only when Function is set to 'PS'.) | <ul style="list-style-type: none"> ● CH1: Apply the configuration to Ch1. ● CH2: Apply the configuration to Ch2. ● CH1&CH2: Apply the configuration to Ch1 and Ch2. |
| | Digital IO-3 Settings | Function setting of pin 3. | |
| | | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid signal is reversed. |
| | | Function | <ul style="list-style-type: none"> ● Off Status: This default function indicates the existing [On/Off] state of the instrument. ● Input: Pin 3 receives the level signal from the outside. ● Output: Pin 3 sends the digital signal (1, 0) to the outside. |
| | | Channel (Displayed only when Function is | <ul style="list-style-type: none"> ● CH1: Apply the configuration to Ch1. ● CH2: Apply the configuration to Ch2. |

| | | |
|-----------------------|---|---|
| | set to 'Off Status'.) | <ul style="list-style-type: none"> ● CH1&CH2: Apply the configuration to Ch1 and Ch2. |
| Digital IO-4 Settings | Function setting of pin 4. | |
| | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid signal is reversed. |
| | Function | <ul style="list-style-type: none"> ● Trigger Out: Configure IO-4 as Trigger Out and enable the triggering output (Trig out) of the List. When the List is triggered to run, IO-4 will output a pulse signal. ● Trigger In: Configure the trigger source of the Oscilloscope function, Data recording, and List function to be external. When the instrument receives an external pulse signal, it will trigger the running of the Oscilloscope function, Data Recording function or List function. ● Input: Pin 4 receives the level signal from the outside. ● Output: Pin 4 sends the digital signal (1, 0) to the outside. |
| | Channel (Displayed only when Function is set to 'Trigger'.) | <ul style="list-style-type: none"> ● CH1: Apply the configuration to Ch1. ● CH2: Apply the configuration to Ch2. ● CH1&CH2: Apply the configuration to Ch1 and Ch2. |
| Digital IO-5 Settings | Function setting of pin 5. | |
| | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid signal is reversed. |
| | Function | <ul style="list-style-type: none"> ● Inhibit-Living: The power supply will be operated in the mode of Living. ● Inhibit-Latch: The power supply will be operated in the mode of Latch. ● Input: Pin 5 receives the level signal from the outside. ● Output: Pin 5 sends the digital signal (1, 0) to the outside. |
| | Channel (Displayed only when Function is set to 'Inhibit'.) | <ul style="list-style-type: none"> ● CH1: Apply the configuration to Ch1. ● CH2: Apply the configuration to Ch2. ● CH1&CH2: Apply the configuration to Ch1 and Ch2. |
| Digital IO-6 Settings | Function setting of pin 6. | |
| | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid signal is reversed. |
| | Function | <ul style="list-style-type: none"> ● Sync On: This default function means that pin 6 performs bi-directional and synchronous control over the turn-on of [On/Off]. ● Input: Pin 6 receives the level signal from the outside. ● Output: Pin 6 sends the digital signal (1, 0) to the outside. |
| Digital IO-7 Settings | Function setting of pin 7. | |
| | Reverse | On/Off, Select Invert or not under the IO Settings. If setting to ON, it means the valid |

| | | |
|--|----------|---|
| | | signal is reversed. |
| | Function | <ul style="list-style-type: none"> ● Sync Off: This default function means that pin 7 performs bi-directional and synchronous control over the turn-off of [On/Off]. ● Input: Pin 7 receives the level signal from the outside. ● Output: Pin 7 sends the digital signal (1, 0) to the outside. |

Signal definition

Digital I/O functions involve input and output levels and pulse signals. The input signal is the control signal provided externally to IT6600, the output signal is the level signal provided externally by IT6600, and the pulse signal is the edge signal switched between high and low levels. The pin signals are defined as follows.

| | | |
|---------------|-------------------|--|
| Input signal | High level signal | Typical: 5V Range: 1.6V-15V Current: $\leq 100\text{mA}$ |
| | Low level signal | Typical: 0V Range: -5V-0.8V Current: $\leq 100\text{mA}$ |
| Output signal | High level signal | Voltage level: 5V |
| | Low level signal | Voltage level: 0V |
| Pulse | Level rise slew | 10us |
| | Level fall slew | 1us |
| | Width | 30us-500us |

Signal Revert

Select Invert or not under the IO Settings menu. If setting to Reverse(Off), it means the default level will be valid. If setting to Reverse(On), it means the valid signal is reversed. For example, the IO-5 pin is inhibit output by default and the high level is valid, when select revert Invert, the low level is valid and the instrument output is disabled.

5.9.2 I/O Control

General Digital I/O Function

- **Digital Input**
Each of the seven pins can be configured as digital input only. Pin 8 is the signal common for the digital input pins. When pins 1 to 7 are configured to Input function, an external signal can be Input to this pin, and the instrument can detect the state of the external signal.
- **Digital Output**
When pins 1 to 7 are configured for the Output function, they can output a high level (False) or low level (True).

- **PWM Output**

Only pins IO-1 and IO-2 can be configured for PWM function, allowing these pins to output PWM signals to external devices. When configured for PWM function, it is necessary to set the values of frequency (Freq) and duty cycle (Duty).

Digital IO-1

IO-1 pin can be set to [PS Clear], [Input], [Output], [PWM]

The default function is to clear the protected state. When the protection occurs, the protection state can be cleared through this pin, so that the instrument can continue to output normally.

Digital IO-2

IO-2 pin can be set to [PS], [Input], [Output], [PWM]

The default function is protection state indicator. IO-2 pin will output high or low level based on whether the instrument is under protection or not. Under normal conditions (Not under protection), and when pin 2 is under default setting (Not Invert), pin 2 outputs high level; when the instrument is under protection, pin 2 outputs low level. When pin 2 is set to Invert, the output level is completely opposite.

Digital IO-3

IO-3 can be set to [OnOff Status], [Input], [Output]

The default function is to indicate the output state of the power supply, in case of output is On, output 5V, otherwise, output 0V.

When pin 3 is set to Invert, the output level is completely opposite.

Digital IO-4

IO-4 can be set to [Trigger-in], [Trigger-out], [Input],[Output]

- [Trigger-in]: The input trigger signal, the pulse signal sent to the IO-4 pin can be used as the trigger source.

Configure the trigger source of the Oscilloscope function, Data recording, and List function to be external. When the instrument receives an external pulse signal, it will trigger the running of the Oscilloscope function, Data Recording function or List function.

- [Trigger-out]: Configure IO-4 as Trigger Out and enable the triggering output (Trig out) of the List. When the List is triggered to run, IO-4 will output a pulse signal.

Digital IO-5

IO-5 pin can be set to [Inhibit-latch], [Inhibit-living], [Input], [Output]

The default function is inhibit output. When the IO pin is configured for a Inhibit function and the level signal is low, the output of the machine is forbidden.

Inhibit function has two mode: Latch and Living.

- Living: When input an inhibit signal and the instrument output is turned OFF. The status bar of the LCD screen displays INH warning icon and the output is marked as OFF. If power supply output is ON state before, the ON/OFF button will be lit. When the input signal undoes, the output returns to normal. This function can be used to control the output of the power supply.

- **Latch:** When input an inhibit signal and the instrument output is turned OFF. The ON/OFF button will be lighted off, the status bar of the LCD screen displays INH warning icon. In this case, user need to remove the input signal and press [Shift]+[Esc] to cleare protection, then manually turn on [On/Off] again.


Digital IO-6

IO-6 pin can be set to[Sync-on], [Input], [Output]

The default function is used to control and monitor the status of the instrument output On. When the power supply output is off, sending a pulse signal to pin 6 will turn the power supply output on. Additionally, when the power supply output changes from off to on, pin 6 will generate a pulse signal as feedback. This function is mainly used to synchronize the output on of multiple instruments.

Taking three instruments as an example, the operation is as below:

1. Go to the **System**→**IO Config**→**Digital IO-6 Settings** menu.
2. Set pin 6's function of three instruments to **Reverse-Off** and **Sync-On**.
3. Referring to the figure below, connect pin 6 of three instruments.

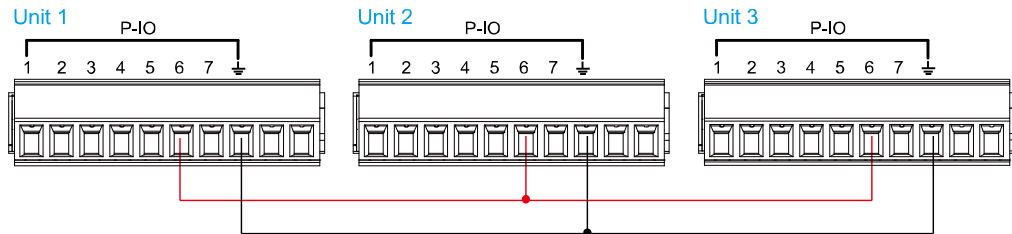

4. Press the **[On/Off]** key of either instrument to switch the output from the Off state to the On state. At this time, the output of the other two instruments will also be turned on synchronously.


Digital IO-7

IO-7 can be set to [Sync-off], [Input], [Output]

The default function is used to control and monitor the status of the instrument output Off. When the power supply output is on, sending a pulse signal to pin 7 will turn the power supply output off. Additionally, when the power supply output changes from on to off, pin 7 will generate a pulse signal as feedback. This function is mainly used to synchronize the output off of multiple instruments.

Taking three instruments as an example, the operation is as below:

1. Go to the **System**→**IO Config**→**Digital IO-7 Settings** menu.
2. Set pin 7's function of three instruments to **Reverse-Off** and **Sync-Off**.
3. Referring to the figure below, connect pin 7 of three instruments.

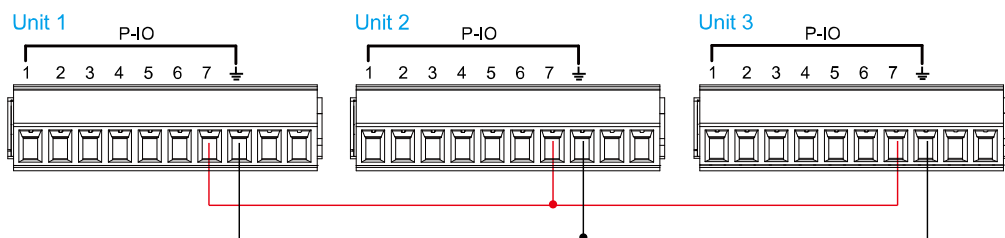

4. Press the **[On/Off]** key of either instrument to switch the output from the On state to the Off state. At this time, the output of the other two instruments

will also be turned off synchronously.

5.10 Analogue Function (Ext-Program) (Optional)


The interface expansion slot provided on the rear panel of the IT6600 series. This function is not standard with the instrument and is optional for users.

When the interface card selected by the user is RS232+Analog interface (IT-E177), the analog interface can realize the external analog function.

- Remotely control voltage and current values.
- Remotely control voltage and current upper limit values.
- Remotely control voltage and current lower limit values.
- Remote monitoring of output voltage/current measurement.

Analog Card Interface Introduction

The pins description is as below.

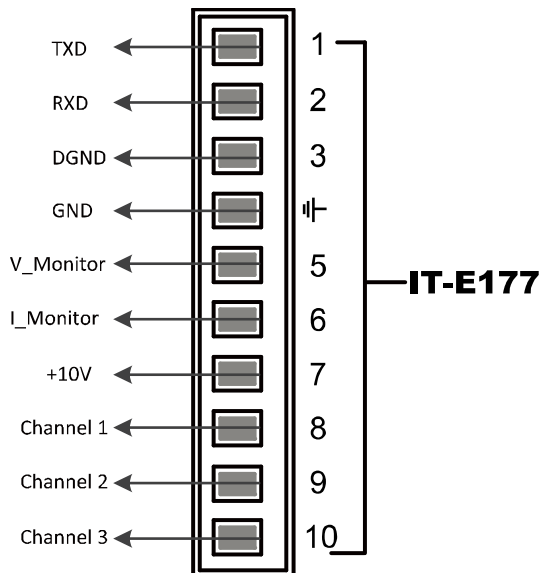

| Pins | Name | Description |
|-------|-----------|---|
| 4 pin | GND | Ground for analog inputs and outputs. |
| 5 pin | V_Monitor | Voltage monitor signal. |
| 6 pin | I_Monitor | Current monitor signal. |
| 7 pin | +10V | The +10V reference voltage output by the power supply can be connected to a resistance subdivision for analog control. |
| 8 pin | Channel 1 | The setting for the output voltage/current value corresponds to Volt Set/Curr Set in the menu. <ul style="list-style-type: none"> ● CV priority: Specify the value of Vs. ● CC priority: Specify the value of Is. |
| 9 pin | Channel 2 | The setting for the voltage/current upper limit corresponds to Volt High/Curr Limit+ in the menu. <ul style="list-style-type: none"> ● CV priority: Specify the value of the current upper limit I+. ● CC priority: Specify the value of the voltage upper limit Vh. |

| Pins | Name | Description |
|--------|-----------|--|
| 10 pin | Channel 3 | The setting for the voltage/current lower limit corresponds to Volt Low/Curr Limit- in the menu. <ul style="list-style-type: none"> ● CV priority: Specify the value of the current lower limit I-. ● CC priority: Specify the value of the voltage lower limit Vl. |

Enable/disable analog control

The user needs to select the corresponding function settings in the System menu. The detailed parameter description is as below.

| External Program | External analog function.(External analog interface is optional.) | |
|-----------------------------------|---|---|
| | Status | Set the On/Off state. |
| | Channel | Select the analog control channel. |
| Displayed when CV is prioritized. | Volt Set Mx | Indicates the slew factor of Volt Set. |
| | Volt Set Mb | Indicates the offset of Volt Set. |
| | Curr Limit+ Mx | Indicates the slew factor of Curr Limit+. |
| | Curr Limit+ Mb | Indicates the offset of Curr Limit+. |
| | Curr Limit- Mx | Indicates the slew factor of Curr Limit-. |
| | Curr Limit- Mb | Indicates the offset of Curr Limit-. |
| Displayed when CC is prioritized | Curr Set Mx | Indicates the slew factor of Curr Set. |
| | Curr Set Mb | Indicates the offset of Curr Set. |
| | Volt High Set Mx | Indicates the slew factor of Volt Limit+. |
| | Volt High Set Mb | Indicates the offset of Volt Limit+. |
| | Volt Low Set Mx | Indicates the slew factor of Volt Limit-. |
| | Volt Low Set Mb | Indicates the offset of Volt Limit-. |

- Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
- Press the up/down key or rotate the knob to find **Source->External program** menu.
 - Set the Set Mx, Set Mb, Limit+ Mx, Limit+ Mb, Limit- Mx and Limit- Mb in sequence, and press **[Enter]** to confirm.
 - Press the up/down key to move the cursor to the **Status** function setting and press the **[Enter]** key to confirm. Rotate the knob to select On to turn on the external analog function.
- Press **[Esc]** to exit.

Analog Conversion Relationship Introduction

The external analog has three channels, and the parameter configuration for each channel follows a linear function $y=kx+b$. The parameter explanations are as follows:

- Independent variable x: The actual input voltage value of the external analog channel.
- Slew factor k: Same as Mx in the menu, set by the user.
- Offset b: Same as Mb in the menu, set by the user.
- y: The actual output value of the instrument. (Voltage when CV is prioritized, current when CC is prioritized)

Taking the **Channel 1**(Volt Set/Curr Set) program setting as an example, the user needs to convert the M_x and M_b values based on the formula below. And set these two values respectively through the front panel keys.


NOTE

The principle of parameter setting of Channel 1 and Channel 2 and Channel 3 is the same, so the description will not be repeated.

- CV priority

$$M_x = \frac{(V_{out2} - V_{out1})}{(V_{in2} - V_{in1})}$$

$$M_b = V_{out2} - V_{in2} \times M_x$$

- CC priority

$$M_x = \frac{(I_{out2} - I_{out1})}{(V_{in2} - V_{in1})}$$

$$M_b = I_{out2} - V_{in2} \times M_x$$


Formula parameter descriptions:

| Name | Description |
|-------|---|
| Vin1 | Indicates the minimum voltage input to pin 8. The setting range is from -10V to 10. |
| Vin2 | Indicates the maximum voltage input to pin 8. The setting range is from -10V to 10, and $V_{in2} > V_{in1}$. |
| Vout1 | The minimum value of the output voltage in CV priority mode. |
| Vout2 | The maximum value of the output voltage in CV priority mode, and $V_{out2} > V_{out1}$. |
| Iout1 | The minimum value of the output current in CC priority mode. |
| Iout2 | The maximum value of the output current in CC priority mode, and $I_{out2} > I_{out1}$. |

Analog Control

The following is an example of how to connect and use the voltage and current control in CC priority mode.

1. Refer to the figure below to complete the pin connection.

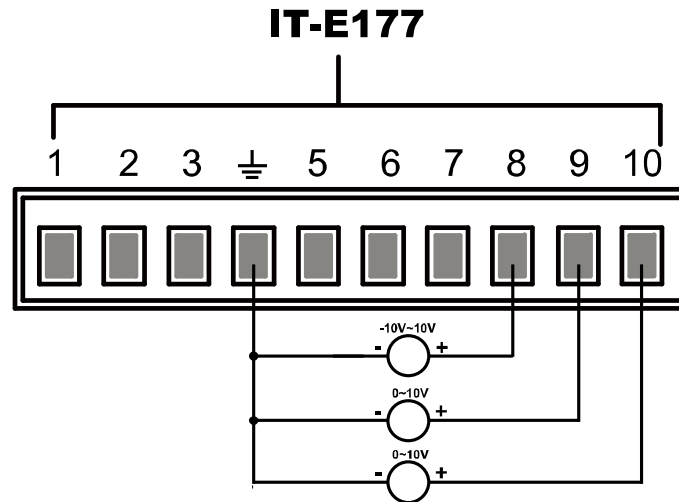

2. Calculate the **Mx** and **Mb** under the Curr Set, Volt Limit+, Volt Limit- menus according to the above formulas. The sample data used in this manual is shown in the table below.

| Pin input voltage | | Power supply output voltage/current | Mx | Mb | Description |
|-------------------|------------|-------------------------------------|----|----|--|
| 8 pin | Vin1 = -10 | lout1=-120A | 12 | 0 | By inputting a voltage of -10V to 10V to pin 8, the actual output current I_s is controlled from -120A to 120A. |
| | Vin2 = 10 | lout2=120A | | | |
| 9 pin | Vin1 = 0 | V+out1 = 0 | 40 | 0 | By inputting a voltage of 0V to 10V to pin 9, the actual output voltage upper limit V+ is controlled from 0 to 400V. |
| | Vin2 = 10 | V+out2 = 400 | | | |
| 10 pin | Vin1 = 0 | V-out1 = 0 | 1 | 0 | By inputting a voltage of 0V to 10V to pin 10, the actual output voltage lower limit V- is controlled from -0 to 10V. |
| | Vin2 = 10 | V-out2 = 10 | | | |

3. Set Mx and Mb of the corresponding pins.
- 1) Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
 - 2) Press the up/down key or rotate the knob to find **Source->External program** menu.
 - 3) Set the Curr Set Mx, Curr Set Mb, Volt High Set Mx, Volt High Set Mb, Volt Low Set Mx and Volt Low Set Mb in sequence, and press **[Enter]** to confirm.
 - 4) Press the up/down key to move the cursor to the **Status** function setting and press the **[Enter]** key to confirm. Rotate the knob to select On to


turn on the external analog function.

4. The input for control **pin 8** is -10V to 10V, the input for control **pin 9** is 0V to 10V, and the input for control **pin 10** is 0V to 10V.

For example, when the input voltage of Pin 8 is 1V, the setting value of the output current of this instrument is 12A; when the input voltage of Pin 9 is 5V, the setting value of the voltage upper limit **V+** of this instrument is 200V; when the input voltage of Pin 10 is 8V, the setting value of the voltage lower limit **V-** of this instrument is 8V.

Voltage and current monitoring

The analog interface can monitor the existing output voltage and output current. Connect a digital voltmeter between Pin 5 and Pin 6 of the analog interface and ground wire 4. The voltage reading from 0 to 10V corresponds to the zero to full-scale voltage/current setting of the instrument. The connection diagram is as shown below.

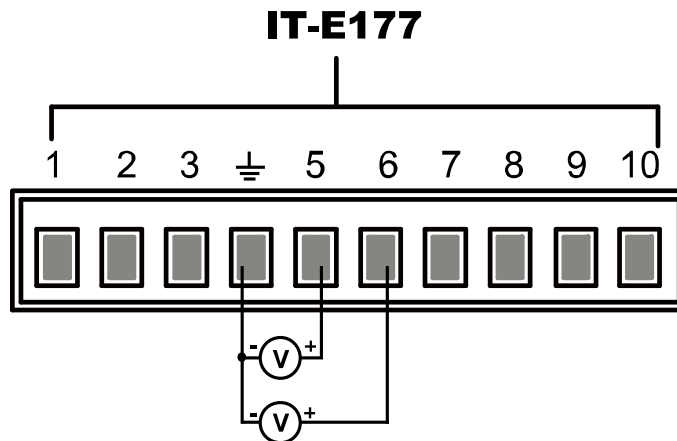





5.11 Redundant function

The redundant function of IT6600C allows observing the status of each cabinet and single unit in parallel mode. When a unit fails, the IT6600C power supply system will automatically identify it, allow the redundant unit to quit the test, and deploy it within the total capacity range to ensure the external output of the entire system.

This means that even if one of the units fails, the IT6600C power system will continue to provide full power to the bus as long as the remaining power can meet the test needs. We call it 100% power availability and it's especially suitable for applications with high reliability requirements of power supply.

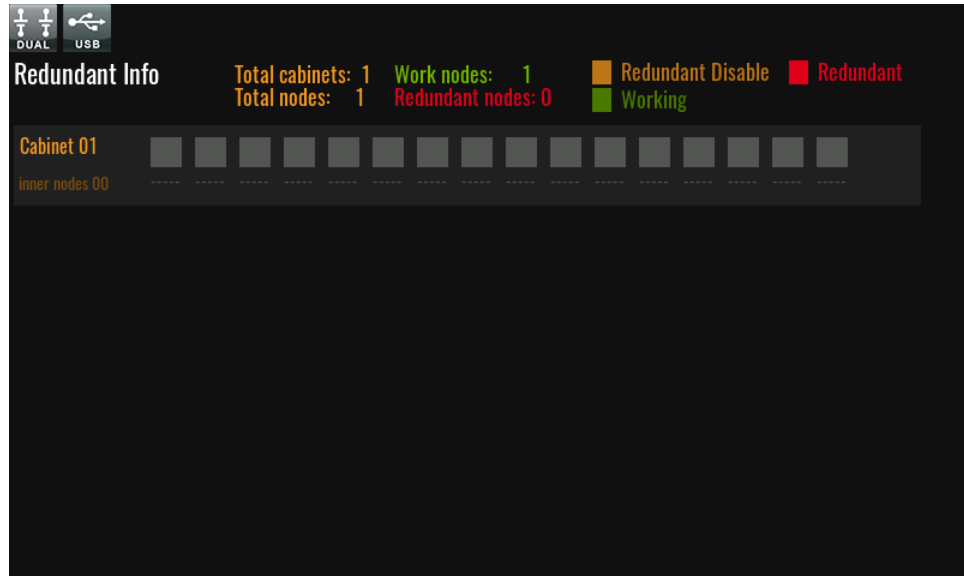Click Off Line on the Menu screen to enter the redundant interfaces.



- Total cabinets: total number of cabinets.
- Total nodes: total number of nodes, i.e., total number of machines in parallel.
- Work nodes: The number of working nodes, i.e., the number of machines that are working properly.
- Redundant nodes: The number of redundant nodes, i.e., the number of machines that have failed.
- Redundant Disable: indicates that the redundant function of the current node has been disabled. The current node displays as .
- Redundant: indicates that the machine in the current node has malfunctioned. The current node displays as .
- Working: indicates that the machine in the current node is operating normally. The current node displays as .
- Inner nodes: the number of internal nodes, i.e. the number of machines contained in a single cabinet.

WARNING

After the redundant function is enabled, the IT6600C power system adopts a **1+X redundant architecture**. Even if multiple units fail, the system can continue to operate normally as long as at least **one unit** remains functional. However, please note that the output power will decrease proportionally based on the number of available units.

Customers should verify whether the remaining output power is sufficient to meet testing requirements in the event of unit failures. For example, if the system consists of four units and three units fail, the remaining one unit can still maintain operation, but the output power will be only **25%** of the original total.

Enable/Disable Redundant function

1. Click on **System** in the menu interface to enter the system menu interface.
2. Select **Source -> Redundant Setting** from the system menu.

- Click the setting located to the right of **Status**, and choose either **On** or **Off** from the dropdown menu.



Chapter6 Measurement Functions

This chapter describes the characteristics and operations of the basic metering function of IT6600 series source.

6.1 Meter Mode

In the **Menu** display interface, click **Meter** to enter the metering interface. See the figure below.



| No. | Name | Description |
|-----|----------------------------------|--|
| 1 | Power status bar | Displays the present output status. |
| 2 | CH1 status bar | Displays the output status of power channel 1. |
| 3 | CH2 status bar | Displays the output status of power channel 2. |
| 4 | Output values view area for CH1 | Displays the present output voltage, current and power values. |
| 5 | Setting values view area for CH1 | <ul style="list-style-type: none"> When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed. When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed. |
| 6 | Output values view area for CH2 | Displays the present output voltage, current and power values. |


- 7 Setting values view area for CH2
- When CV is prioritized, the voltage setting value, current upper limit value, current lower limit value, power upper limit value, and power lower limit value are displayed.
 - When CC is prioritized, the current setting value, voltage upper limit value, voltage lower limit value, power upper limit value, and power lower limit value are displayed.

6.2 Oscilloscope Mode

IT6600 series source has the function of displaying the waveform based on sampling data. The user can select to display or hide the voltage and current waveform of the input unit. Only the necessary waveform is displayed, which can facilitate observation. The waveform display interface includes the vertical axis and horizontal axis.

Introduction of Waveform Display interface

In the **Menu** display interface, click **Scope** to enter the waveform interface. See the figure below.

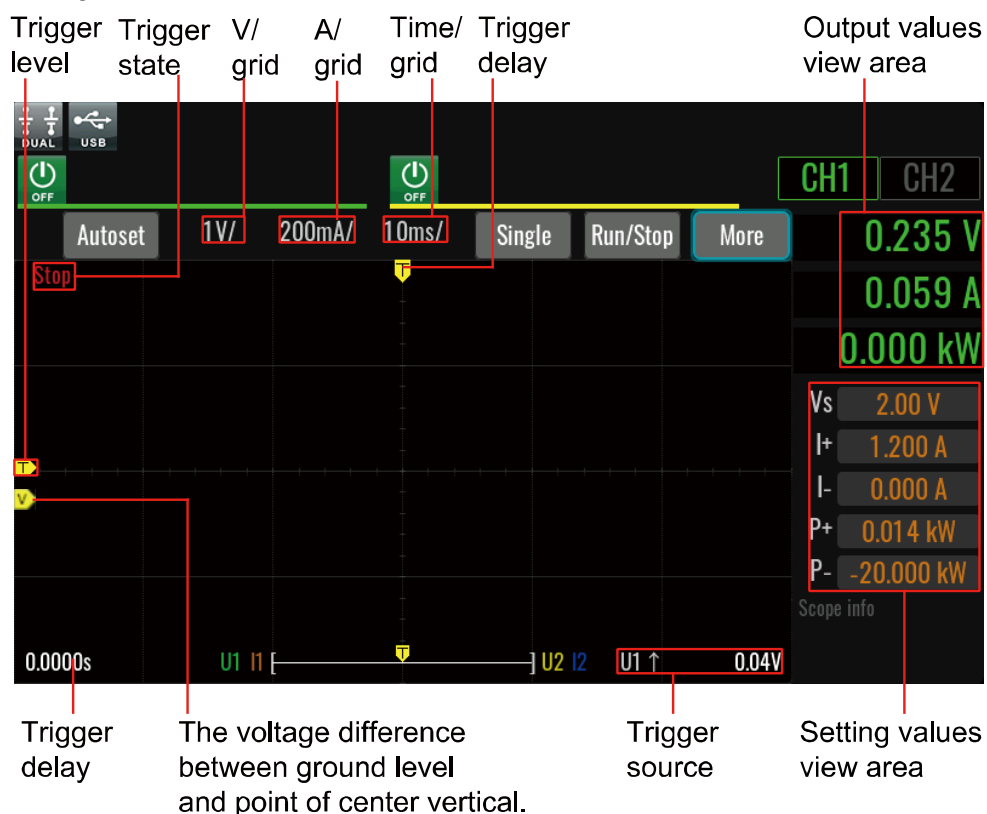

The trigger status is described as follows:

| Trigger status | Instruction |
|----------------|--|
| Auto | Select the trigger mode as "Auto," with the trigger status displayed as "Auto" when triggered. |
| Roll | Select the trigger mode as "Auto," with the trigger status displayed as "Roll" when not triggered. |
| Trig | Select the trigger mode as "Normal," with the trigger status |

| | |
|-------|--|
| | displayed as "Trig" when triggered. |
| Ready | Select the trigger mode as "Normal," with the trigger status displayed as "Ready" when not triggered. |
| Stop | When the "Stop" key in the waveform display interface is pressed, the trigger status Stop will be displayed. |

Description of keys on the waveform display interface:

- AutoSet: Automatically adjust the appropriate time base, voltage/current scale, and restore the trigger level and trigger delay to default values.
- Voltage/Current/Time: Adjust voltage/current/time base range.
- Single: Single measurement key: when single measurement is enabled in the Stop status, the stop status is enabled again after one measurement based on the current data updating rate. When single measurement is enabled in the Ready status, the instrument immediately restarts one measurement and then enters the Stop status.
- Run/Stop: press the corresponding soft key to run or stop the waveform status.
- More: Advanced configuration options for oscilloscope function.

| Parameter | Description |
|----------------|---|
| Trigger source | <p>Select trigger source, Voltage, Current and External can be select.</p> <ul style="list-style-type: none"> ● Voltage trigger. When the DC terminals detect that the voltage reaches the trigger voltage setting value and is within the range of the upper and lower trigger limits, a data recording operation is triggered. <ul style="list-style-type: none"> ➢ Trig Level: Trigger threshold. ➢ Edge: Select trigger edge: rising edge (Rise), descending edge (Fall) or either edge (Both). ➢ Trig High: Trigger upper limit value. ➢ Trig Low: Trigger lower limit value. ● Current trigger. When the DC terminals detect that the current reaches the trigger current setting value and is within the range of the upper and lower trigger limits, a data recording operation is triggered. <ul style="list-style-type: none"> ➢ Trig Level: Trigger threshold. ➢ Edge: Select trigger edge: rising edge (Rise), descending edge (Fall) or either edge (Both). ➢ Trig High: Trigger upper limit value. ➢ Trig Low: Trigger lower limit value. ● External: Indicates the trigger occurs via the pin 4 of the digital I/O interface (P-IO). For details, see 5.9 Digital I/O Function. |
| Trigger mode | Auto and Normal can be select. |
| Print data | <p>Save the data.</p> <ul style="list-style-type: none"> ● Depth: data record depth. ● Algorithm: with the option of Normal or Peak. |

| | |
|----------------|--|
| Line selection | Select the displayed curve, which is used to select whether to display the voltage/current waveform of the corresponding channel. Up to 4 oscillographic data curves can be displayed. |
|----------------|--|

Trigger waveform

When the specified trigger conditions are satisfied, the trigger waveform will be displayed. The triggering time is the trigger point, generally on the middle of the screen. When the trigger point is reached, the screen will display the waveform from left to right over time. The user should set the following parameters before using the trigger function.

- **Trigger mode**

The trigger mode refers to the condition to update the contents on the screen. It is divided into the Auto mode and Normal mode. In the Auto mode, the displayed waveform will be updated when triggering occurs in the suspension time; otherwise, the displayed waveform will be updated automatically.

In the Normal mode, the displayed waveform will be updated in the case of triggering and not updated in the case of no triggering.

- **Trigger source**

The trigger source is used for generating trigger conditions.

- **Trigger edge**

The edge refers to the change of the signal from low level to high level (rising edge) or from high level to low level (falling edge). The edge used as a trigger condition is referred to as the trigger edge.

- **Trigger level**

The trigger level refers to the level which the trigger edge passes through. If the signal of the trigger source passes through the set trigger level according to the specified trigger edge, triggering occurs.

When "U↑" is selected for editing, you can adjust the trigger level using the knob, number keys, or arrow keys. In this case, the trigger level can be changed by rotating the knob and you can observe trigger level changes on the screen.

Horizontal Control and Vertical Control

- **Vertical calibration**

When V/grid or A/grid is selected, you can rotate the knob to set the voltage or current range of each interval.

- **Horizontal calibration**

When Time/grid is selected, you can rotate the knob to adjust the horizontal scale (scanning speed). When the horizontal (time/scale) setting is changed by rotating the knob, you can observe the change of time/scale on the screen.

- **Trigger delay**

You can adjust the trigger delay using the editing box (knob/directional keys/numeric keys) or by horizontal sliding. The default trigger delay is 0,

which positions the trigger point (📌) in the middle of the waveform display area. When the trigger delay value is positive, the trigger point moves to the left; when it is negative, the trigger point moves to the right.

Print data

In the **More** menu, users can select the **Print Data** item and select the data logging mode. Data of oscilloscope interface will be recorded to U disk.


Print data mode:

- Off: turn off the print data function.
- Post: Record the position data of the waveform.
- Raw: The recorded data is original data, The default data sampling interval is 10us.
- Both: Post and Raw, record two data file.

6.3 Recorder Function

The data recording function allows you to observe and record output status data for a long time. On the recorder interface, you can select a maximum of six data curves to be displayed.

In the **Menu** display interface, click **Recorder** to enter the data recording function interface. See the figure below.

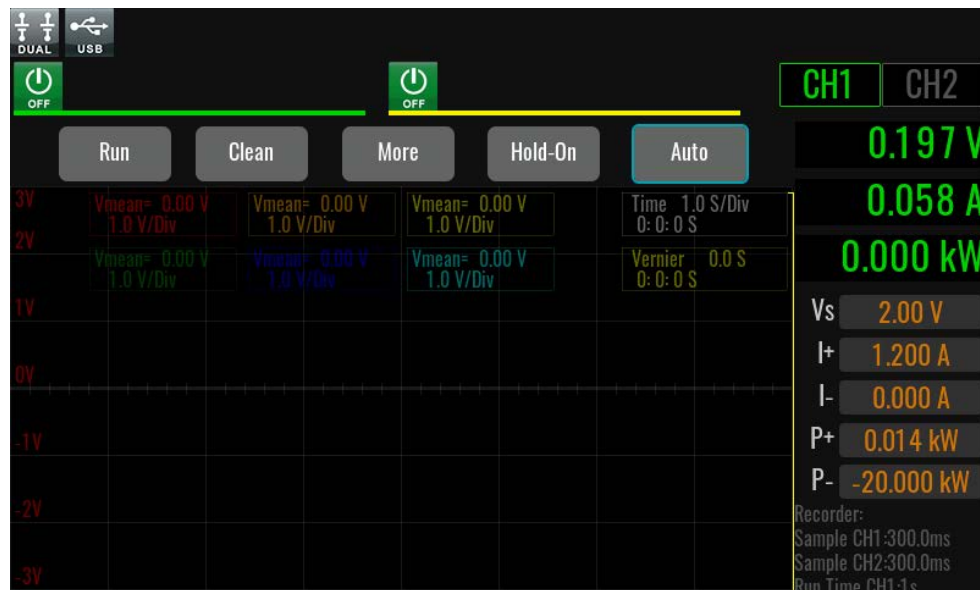

- Run/Stop: Run/Stop refresh data.
- Clean: Clean all of data curve.
- More: Enter to the advanced menu to set more parameters.


| Parameter | Description |
|-----------------|---|
| Viewing control | Select the number of data curves currently displayed and the corresponding parameters. Up to six curves can be displayed, with optional parameters including Vmean, Vmin, Vmax, Imean, Imin, Imax, Pmean, Pmin, Pmax. |

| | |
|----------------------|---|
| Record objects(Dlog) | <p>Select the data objects to be recorded.</p> <ul style="list-style-type: none"> ● Run state: Enable or disable storage status. If disabled, all data will not be saved or displayed. ● Voltage: Enable or disable voltage storage. ● Current: Enable or disable current storage. ● Power: Enable or disable power storage. |
| Trigger settings | <p>Select the trigger source of the recorder function, including Immediate, Manual, Bus, Voltage, Current, and External.</p> <ul style="list-style-type: none"> ● Immediate: Perform a trigger operation immediately. ● Manual: Indicates the trigger occurs when the [Shift]+[5](Trigger) keys are pressed from the front panel. ● Bus: Bus trigger. When the trigger command *TRG is received, the instrument generates a trigger. ● Voltage trigger. When the DC terminals detect that the voltage reaches the trigger voltage setting value and is within the range of the upper and lower trigger limits, a data recording operation is triggered. <ul style="list-style-type: none"> ➢ Trig Level: Trigger threshold. ➢ Edge: Select trigger edge: rising edge (Rise), descending edge (Fall) or either edge (Both). ➢ Trig High: Trigger upper limit value. ➢ Trig Low: Trigger lower limit value. ● Current trigger. When the DC terminals detect that the current reaches the trigger current setting value and is within the range of the upper and lower trigger limits, a data recording operation is triggered. <ul style="list-style-type: none"> ➢ Trig Level: Trigger threshold. ➢ Edge: Select trigger edge: rising edge (Rise), descending edge (Fall) or either edge (Both). ➢ Trig High: Trigger upper limit value. ➢ Trig Low: Trigger lower limit value. ● External: Indicates the trigger occurs via the pin 4 of the digital I/O interface (P-IO). For details, see 5.9 Digital I/O Function. |
| Run time | <p>This parameter indicates the time for data recording (unit: s), namely, the data recording will be completed in Y seconds and be ready for the next data record. The input range supported by the instrument is: 0-9999999s.</p> |
| Sampling period | <p>This parameter indicates the data sampling interval (unit: ms), that is, the test data is recorded once every X seconds. The input range supported by the instrument is: 0.1ms-1000ms.</p> |
| File format | <p>Select the file format, include Tdms and CSV.</p> |

- Hold-On/Hold-Off: Pause screen data refresh (for data observation)/ Start dynamically observing the data
- Auto: Automatically adjusts the scale of the appropriate vertical axis.
- Time: The time value of each of the horizontal coordinates, unit is s/Div
- Vernier: Position information of the vernier caliper.

6.4 Query the Energy

IT6600 series power supply provides the energy statistics function, including voltage, frequency and power of each phase as well as current electric energy, stage electric energy and total electric energy. In the **Menu** display interface, click **AC Meter** to enter the energy query interface.

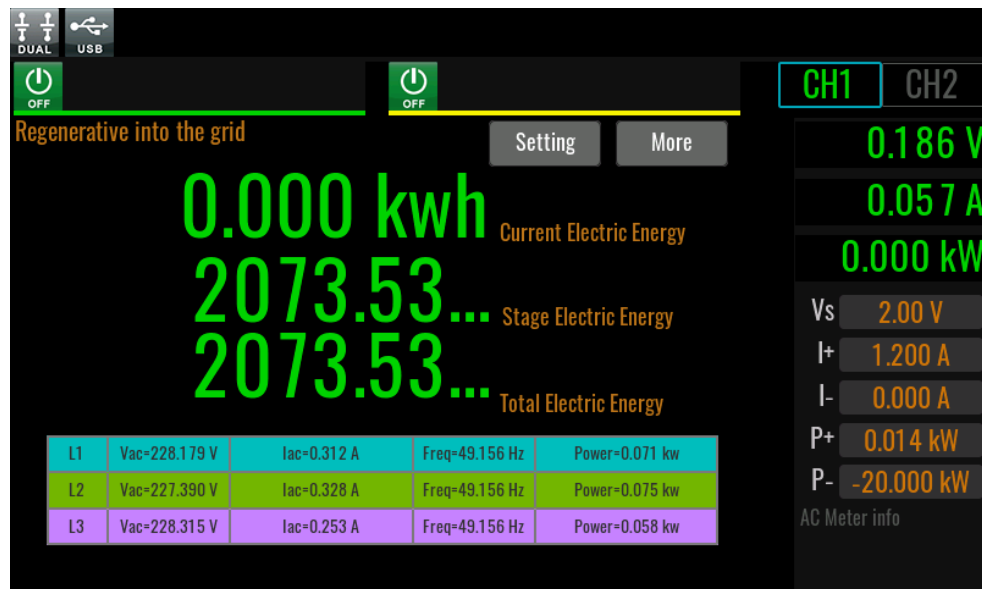

- Setting: enter the setting interface and select Clear to zero the current electric energy and stage electric energy.
- More: enter the **More** interface to query more historical information.

Chapter7 Technical Specifications

This chapter will introduce the main technical parameters of this power, such as rated voltage/current/power and so on. Besides, this part will introduce the working environment and storage temperature.

7.1 Supplemental characteristics

Recommended calibration frequency: once a year

Cooling style: fans

7.2 Main technical parameters

IT6642C-1200-200

| Parameter | | IT6642C-1200-200 | |
|----------------------|------------------------------------|------------------------------|-------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -200A~200A |
| | | 2-channel mode/Series mode | -100A~100A |
| | Power | Each channel | -21kW~21kW |
| | | Total | -42kW~42kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.6Ω |
| | | Parallel mode | 0~0.3Ω |
| | | Series mode | 0~1.2Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.046~7500Ω |
| Parallel mode | | 0.023~7500Ω | |
| Series mode | | 0.092~7500Ω | |
| Line Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.01%FS | |
| Load Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.015%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.1%FS |
| | Vrms | 20Hz-20MHz | ≤0.02%FS |
| | Irms | 20Hz-300KHz | ≤0.1%FS |
| Setup Temperature | Voltage | ≤15PPM/°C | |

| | | | |
|--|---|---------------------------------------|----------------------------|
| Coefficient | Current | $\leq 30\text{PPM}/^{\circ}\text{C}$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15\text{PPM}/^{\circ}\text{C}$ | |
| | Current | $\leq 30\text{PPM}/^{\circ}\text{C}$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1\text{ms}$ | |
| Rise Time (full load) *4 | Voltage | $\leq 1\text{ms}$ | |
| Fall Time (no load) *3 | Voltage | $\leq 1\text{ms}$ | |
| Fall Time (full load) *4 | Voltage | $\leq 1\text{ms}$ | |
| Rise Time (full current) *5 | Current | $\leq 350\mu\text{s}$ | |
| Fall Time (full current) *5 | Current | $\leq 350\mu\text{s}$ | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | $\leq 200\mu\text{s}$ | |
| AC Input | Input voltage *6 | Three phase + PE | 21 kW Max. @180-264V-Input |
| | | | 42 kW Max. @342-528V-Input |
| | Maximum Input Current | 73A(per phase)@200Vac, 3 ϕ input | |
| | | 77A(per phase)@380Vac, 3 ϕ input | |
| | | 61A(per phase)@480Vac, 3 ϕ input | |
| Maximum Input Apparent Power | 45.4kVA | | |
| Frequency | 47Hz ~ 63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | $\leq 0.005\% + 0.005\%\text{FS}$ | |
| | Current | $\leq 0.01\% + 0.01\%\text{FS}$ | |
| Setup Stability-8h | Voltage | $\leq 0.005\% + 0.005\%\text{FS}$ | |
| | Current | $\leq 0.01\% + 0.01\%\text{FS}$ | |
| Readback Stability-30min | Voltage | $\leq 0.005\% + 0.005\%\text{FS}$ | |
| | Current | $\leq 0.01\% + 0.01\%\text{FS}$ | |
| Readback Stability-8h | Voltage | $\leq 0.005\% + 0.005\%\text{FS}$ | |
| | Current | $\leq 0.01\% + 0.01\%\text{FS}$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 58.4 $\mu\text{F}/\text{CH}$ | |
| Min. operating voltage | $\leq 0.5\%\text{FS}$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}\text{C} \sim 70^{\circ}\text{C}$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 1200\text{Vdc}$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0 ~ 50 $^{\circ}\text{C}$ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 483mm(W)* 151.3mm(H)* 831.6mm(D) | | |
| Weight(net) | (48.5 \pm 1) kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{\text{set}} - \Delta I) - R_{\text{set}}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30\text{V}$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC \pm 10%, such as the need for 480VAC \pm 10% voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT6684C-1200-400

| Parameter | | IT6684C-1200-400 | |
|----------------------|------------------------------------|------------------------------|-------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -400A~400A |
| | | 2-channel mode/Series mode | -200A~200A |
| | Power | Each channel | -42kW~42kW |
| | | Total | -84kW~84kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.3Ω |
| | | Parallel mode | 0~0.15Ω |
| | | Series mode | 0~0.6Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.023~7500Ω |
| Parallel mode | | 0.012~7500Ω | |
| Series mode | | 0.046~7500Ω | |
| Line Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.01%FS | |
| Load Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.015%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |

| | | | |
|---|---|----------------------------------|----------------------------|
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.11%FS |
| | Vrms | 20Hz-20MHz | ≤0.022%FS |
| | Irms | 20Hz-300KHz | ≤0.11%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤1ms | |
| Rise Time (full load) *4 | Voltage | ≤1ms | |
| Fall Time (no load) *3 | Voltage | ≤1ms | |
| Fall Time (full load) *4 | Voltage | ≤1ms | |
| Rise Time (full current) *5 | Current | ≤350us | |
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 42 kW Max. @180-264V-Input |
| | | | 84 kW Max. @342-528V-Input |
| | Maximum Input Current | 146A(per phase)@200Vac, 3ø input | |
| | | 154A(per phase)@380Vac, 3ø input | |
| | | 122A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 90.8kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 116.8uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±1200Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 550.0mm(W)* 907.64mm(H)*841.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 186kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/Rset)$

- ΔI – Rset. where V is the external voltage, Rset is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66126C-1200-600

| Parameter | | IT66126C-1200-600 | |
|----------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -600A~600A |
| | | 2-channel mode/Series mode | -300A~300A |
| | Power | Each channel | -63kW~63kW |
| | | Total | -126kW~126kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.2Ω |
| | | Parallel mode | 0~0.1Ω |
| | | Series mode | 0~0.4Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.016~7500Ω |
| Parallel mode | | 0.008~7500Ω | |
| Series mode | | 0.031~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |

| | | | |
|---|--|----------------------------|---|
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.12\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.024\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.12\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^\circ C$ | |
| | Current | $\leq 30PPM/^\circ C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^\circ C$ | |
| | Current | $\leq 30PPM/^\circ C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Rise Time (full current) *5 | Current | $\leq 350us$ | |
| Fall Time (full current) *5 | Current | $\leq 350us$ | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | $\leq 200us$ | |
| AC Input | Input voltage *6 | Three phase + PE | 63 kW Max. @180-264V-Input 126 kW Max. @342-528V-Input |
| | | Maximum Input Current | 219A(per phase) @200Vac, 3 ϕ input 230A(per phase) @380Vac, 3 ϕ input 182A(per phase) @480Vac, 3 ϕ input |
| | Maximum Input Apparent Power | 136.2kVA | |
| | Frequency | 47Hz~63Hz | |
| | Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 175.2uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^\circ C \sim 70^\circ C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 1200Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50 $^\circ C$ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 550.0mm(W)* 907.64mm(H)*841.1mm(1008.1mm | | |

| | |
|--------------|--------------------------------|
| | including protective cover)(D) |
| Weight(net) | 237kg |

- *1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.
- *2. This specification was tested under test conditions with an output voltage of $\geq 30V$.
- *3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.
- *7. Power factor of 0.99 at 50% of rated power and above at nominal input.
- *8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66168C-1200-800

| Parameter | | IT66168C-1200-800 | |
|----------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -800A~800A |
| | | 2-channel mode/Series mode | -400A~400A |
| | Power | Each channel | -84kW~84kW |
| | | Total | -168kW~168kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.15Ω |
| | | Parallel mode | 0~0.075Ω |
| | | Series mode | 0~0.3Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.012~7500Ω |
| Parallel mode | | 0.006~7500Ω | |
| Series mode | | 0.023~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |

| | | | |
|---|--|---|-----------------------------|
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.13\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.026\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.13\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Rise Time (full current) *5 | Current | $\leq 350us$ | |
| Fall Time (full current) *5 | Current | $\leq 350us$ | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | $\leq 200us$ | |
| AC Input | Input voltage *6 | Three phase + PE | 84 kW Max. @180-264V-Input |
| | | | 168 kW Max. @342-528V-Input |
| | Maximum Input Current | 292A(per phase) @200Vac, 3 ϕ input | |
| | | 307A(per phase) @380Vac, 3 ϕ input | |
| | | 243A(per phase) @480Vac, 3 ϕ input | |
| Maximum Input Apparent Power | 181.5kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.005\% + 0.005\%FS$ | |
| | Current | $\leq 0.01\% + 0.01\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 233.6uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 1200Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |

| | |
|------------------------|--|
| Working Temperature *8 | 0~50°C |
| IP | IP20 |
| Safety Standard | IEC 61010 |
| Cooling | Air |
| Dimension (mm) | 600.0mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) |
| Weight(net) | 346kg |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66210C-1200-1000

| Parameter | | IT66210C-1200-1000 | |
|-----------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -1000A~1000A |
| | | 2-channel mode/Series mode | -500A~500A |
| | Power | Each channel | -105kW~105kW |
| | | Total | -210kW~210kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.12Ω |
| | | Parallel mode | 0~0.06Ω |
| | | Series mode | 0~0.24Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.01~7500Ω |
| Parallel mode | | 0.005~7500Ω | |
| Series mode | | 0.019~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |

| | | | |
|--|---|----------------------------------|-----------------------------|
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.14%FS |
| | Vrms | 20Hz-20MHz | ≤0.028%FS |
| | Irms | 20Hz-300KHz | ≤0.14%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 105 kW Max. @180-264V-Input |
| | | | 210 kW Max. @342-528V-Input |
| | Maximum Input Current | 364A(per phase)@200Vac, 3ø input | |
| | | 383A(per phase)@380Vac, 3ø input | |
| | | 304A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 226.9kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 292uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, | | |

| | EtherCAT card, Relay cards | |
|-----------------------------------|--|--------------|
| Maximum Working Isolation Voltage | ±1200Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.0mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 397kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66252C-1200-1200

| Parameter | | IT66252C-1200-1200 | |
|---------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -1200A~1200A |
| | | 2-channel mode/Series mode | -600A~600A |
| | Power | Each channel | -126kW~126kW |
| | | Total | -252kW~252kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.1Ω |
| | | Parallel mode | 0~0.05Ω |
| | | Series mode | 0~0.2Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.008~7500Ω |
| Parallel mode | | 0.004~7500Ω | |

| | | Series mode | 0.016~7500Ω |
|--|-----------------------------|----------------------------------|-----------------------------|
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.15%FS |
| | Vrms | 20Hz-20MHz | ≤0.03%FS |
| | Irms | 20Hz-300KHz | ≤0.15%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 126 kW Max. @180-264V-Input |
| | | | 252 kW Max. @342-528V-Input |
| | Maximum Input Current | 437A(per phase)@200Vac, 3ø input | |
| | | 460A(per phase)@380Vac, 3ø input | |
| | | 364A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 272.3kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 350.4uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |

| | | |
|-----------------------------------|---|--------------|
| Command Response Time | 1ms | |
| Storage Temperature | -10°C~70°C | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±1200Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 447kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66294C-1200-1400

| Parameter | | IT66294C-1200-1400 | |
|-------------|---------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -1400A~1400A |
| | | 2-channel mode/Series mode | -700A~700A |
| | Power | Each channel | -147kW~147kW |
| | | Total | -294kW~294kW |

| | | | |
|--|------------------------------------|----------------------------------|-----------------------------|
| | Resistance in series (CV priority) | 2-channel mode | 0~0.086Ω |
| | | Parallel mode | 0~0.043Ω |
| | | Series mode | 0~0.172Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.007~7500Ω |
| | | Parallel mode | 0.004~7500Ω |
| | | Series mode | 0.014~7500Ω |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.16%FS |
| | Vrms | 20Hz-20MHz | ≤0.032%FS |
| | Irms | 20Hz-300KHz | ≤0.16%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 147 kW Max. @180-264V-Input |
| | | | 294 kW Max. @342-528V-Input |
| | Maximum Input Current | 510A(per phase)@200Vac, 3ø input | |
| | | 537A(per phase)@380Vac, 3ø input | |
| | | 425A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 317.7kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full | ~94.5% | |

| | | |
|-----------------------------------|--|--------------|
| | power | |
| | Full voltage and full power | ~95% |
| Output Port Capacitance | 2-channel mode | 408.8uF/CH |
| Min. operating voltage | ≤0.5%FS | |
| Remote Sense Voltage | 1%FS | |
| Command Response Time | 1ms | |
| Storage Temperature | -10°C~70°C | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±1200Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 497kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66336C-1200-1600

| Parameter | | IT66336C-1200-1600 |
|-------------|------------------------------|--------------------|
| Rated value | Series mode | 0~1200V |
| | 2-channel mode/Parallel mode | 0~600V |

| | | | |
|---|------------------------------------|----------------------------------|-----------------------------|
| | Current | Parallel mode | -1600A~1600A |
| | | 2-channel mode/Series mode | -800A~800A |
| | Power | Each channel | -168kW~168kW |
| | | Total | -336kW~336kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.075Ω |
| | | Parallel mode | 0~0.038Ω |
| | | Series mode | 0~0.15Ω |
| Load resistance (CC priority) | 2-channel mode | 0.006~7500Ω | |
| | Parallel mode | 0.003~7500Ω | |
| | Series mode | 0.012~7500Ω | |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.17%FS |
| | Vrms | 20Hz-20MHz | ≤0.034%FS |
| | Irms | 20Hz-300KHz | ≤0.17%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 168 kW Max. @180-264V-Input |
| | | | 336 kW Max. @342-528V-Input |
| | Maximum Input Current | 583A(per phase)@200Vac, 3ø input | |
| | | 613A(per phase)@380Vac, 3ø input | |
| | | 486A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 363kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |

| | | | |
|-----------------------------------|--|----------------|--|
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 467.2uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±1200Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 583kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66378C-1200-1800

| Parameter | | IT66378C-1200-1800 | |
|---|------------------------------------|----------------------------------|-----------------------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -1800A~1800A |
| | | 2-channel mode/Series mode | -900A~900A |
| | Power | Each channel | -189kW~189kW |
| | | Total | -378kW~378kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.067Ω |
| | | Parallel mode | 0~0.034Ω |
| | | Series mode | 0~0.134Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.006~7500Ω |
| Parallel mode | | 0.003~7500Ω | |
| Series mode | | 0.011~7500Ω | |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.18%FS |
| | Vrms | 20Hz-20MHz | ≤0.036%FS |
| | Irms | 20Hz-300KHz | ≤0.18%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 189 kW Max. @180-264V-Input |
| | | | 378 kW Max. @342-528V-Input |
| | Maximum Input Current | 655A(per phase)@200Vac, 3ø input | |
| | | 690A(per phase)@380Vac, 3ø input | |
| 546A(per phase)@480Vac, 3ø input | | | |
| Maximum Input | 408.4kVA | | |

| | | |
|-----------------------------------|---|----------------|
| | Apparent Power | |
| | Frequency | 47Hz~63Hz |
| | Power Factor *7 | 0.99 |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Efficiency | Full current and full power | ~94.5% |
| | Full voltage and full power | ~95% |
| Output Port Capacitance | 2-channel mode | 525.6uF/CH |
| Min. operating voltage | | ≤0.5%FS |
| Remote Sense Voltage | | 1%FS |
| Command Response Time | | 1ms |
| Storage Temperature | | -10°C~70°C |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±1200Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 633kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66420C-1200-2000

| Parameter | | IT66420C-1200-2000 | |
|---|------------------------------------|------------------------------|-----------------------------|
| Rated value | Voltage | Series mode | 0~1200V |
| | | 2-channel mode/Parallel mode | 0~600V |
| | Current | Parallel mode | -2000A~2000A |
| | | 2-channel mode/Series mode | -1000A~1000A |
| | Power | Each channel | -210kW~210kW |
| | | Total | -420kW~420kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.06Ω |
| | | Parallel mode | 0~0.03Ω |
| | | Series mode | 0~0.12Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.005~7500Ω |
| Parallel mode | | 0.003~7500Ω | |
| Series mode | | 0.01~7500Ω | |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.19%FS |
| | Vrms | 20Hz-20MHz | ≤0.038%FS |
| | Irms | 20Hz-300KHz | ≤0.19%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 210 kW Max. @180-264V-Input |

| | | |
|-----------------------------------|------------------------------|---|
| | | 420 kW Max. @342-528V-Input |
| | Maximum Input Current | 728A(per phase)@200Vac, 3ø input |
| | | 766A(per phase)@380Vac, 3ø input |
| | | 607A(per phase)@480Vac, 3ø input |
| | Maximum Input Apparent Power | 453.8kVA |
| Frequency | 47Hz~63Hz | |
| Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS |
| | Current | ≤0.02%+0.02%FS |
| Efficiency | Full current and full power | ~94.5% |
| | Full voltage and full power | ~95% |
| Output Port Capacitance | 2-channel mode | 584uF/CH |
| Min. operating voltage | | ≤0.5%FS |
| Remote Sense Voltage | | 1%FS |
| Command Response Time | | 1ms |
| Storage Temperature | | -10°C~70°C |
| Protective Function | | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection |
| Standard Interface | | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards |
| Maximum Working Isolation Voltage | | ±1200Vdc |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | | 0~50°C |
| IP | | IP20 |
| Safety Standard | | IEC 61010 |
| Cooling | | Air |
| Dimension (mm) | | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) |
| Weight(net) | | 683kg |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC \pm 10%, such as the need for 480VAC \pm 10% voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT6642C-1600-140

| Parameter | | IT6642C-1600-140 | |
|-----------------------------------|------------------------------------|------------------------------|-----------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -140A~140A |
| | | 2-channel mode/Series mode | -70A~70A |
| | Power | Each channel | -21kW~21kW |
| | | Total | -42kW~42kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~1.143Ω |
| | | Parallel mode | 0~0.572Ω |
| | | Series mode | 0~2.286Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.066~7500Ω |
| Parallel mode | | 0.033~7500Ω | |
| Series mode | | 0.131~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.1\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.02\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.1\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Rise Time (full current) *5 | Current | $\leq 350us$ | |

| | | | |
|---|---|---------------------------------|----------------------------|
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 21 kW Max. @180-264V-Input |
| | | | 42 kW Max. @342-528V-Input |
| | Maximum Input Current | 73A(per phase)@200Vac, 3ø input | |
| | | 77A(per phase)@380Vac, 3ø input | |
| | | 61A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 45.4kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 14.6uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±1600Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 483mm(W)* 151.3mm(H)* 831.6mm(D) | | |
| Weight(net) | (48.5±1) kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-

impedance DC Bi-directional source, when the output current makes a step change from $-100\%FS$ to $+100\%FS$ (or $+100\%FS$ to $-100\%FS$), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports $380VAC \pm 10\%$, such as the need for $480VAC \pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds $40^{\circ}C$, the rated current and power decrease by 3% for every $1^{\circ}C$ increase. When the cabinet temperature exceeds $30^{\circ}C$, they decrease by 2% for every $1^{\circ}C$ increase. Both are applicable up to a maximum of $50^{\circ}C$.

IT6684C-1600-280

| Parameter | | IT6684C-1600-280 | |
|-----------------------------------|------------------------------------|------------------------------|------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -280A~280A |
| | | 2-channel mode/Series mode | -140A~140A |
| | Power | Each channel | -42kW~42kW |
| | | Total | -84kW~84kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.572Ω |
| | | Parallel mode | 0~0.286Ω |
| | | Series mode | 0~1.143Ω |
| Load resistance (CC priority) | 2-channel mode | 0.033~7500Ω | |
| | Parallel mode | 0.017~7500Ω | |
| | Series mode | 0.066~7500Ω | |
| Line Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.01%FS | |
| Load Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.015%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.11%FS |
| | Vrms | 20Hz-20MHz | ≤0.022%FS |
| | Irms | 20Hz-300KHz | ≤0.11%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤1ms | |

| | | | |
|--|---|----------------------------------|----------------------------|
| Rise Time (full load) *4 | Voltage | ≤1ms | |
| Fall Time (no load) *3 | Voltage | ≤1ms | |
| Fall Time (full load) *4 | Voltage | ≤1ms | |
| Rise Time (full current) *5 | Current | ≤350us | |
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 42 kW Max. @180-264V-Input |
| | | | 84 kW Max. @342-528V-Input |
| | Maximum Input Current | 146A(per phase)@200Vac, 3ø input | |
| | | 154A(per phase)@380Vac, 3ø input | |
| | | 122A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 90.8kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 29.2uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10℃~70℃ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±1600Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50℃ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 550.0mm(W)* 907.64mm(H)*841.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 186kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC \pm 10%, such as the need for 480VAC \pm 10% voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66126C-1600-420

| Parameter | | IT66126C-1600-420 | |
|----------------------|------------------------------------|------------------------------|------------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -420A~420A |
| | | 2-channel mode/Series mode | -210A~210A |
| | Power | Each channel | -63kW~63kW |
| | | Total | -126kW~126kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.381Ω |
| | | Parallel mode | 0~0.191Ω |
| | | Series mode | 0~0.762Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.022~7500Ω |
| Parallel mode | | 0.011~7500Ω | |
| Series mode | | 0.044~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.12\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.024\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.12\%FS$ |

| | | | |
|--|---|----------------------------------|-----------------------------|
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤1ms | |
| Rise Time (full load) *4 | Voltage | ≤1ms | |
| Fall Time (no load) *3 | Voltage | ≤1ms | |
| Fall Time (full load) *4 | Voltage | ≤1ms | |
| Rise Time (full current) *5 | Current | ≤350us | |
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 63 kW Max. @180-264V-Input |
| | | | 126 kW Max. @342-528V-Input |
| | Maximum Input Current | 219A(per phase)@200Vac, 3ø input | |
| | | 230A(per phase)@380Vac, 3ø input | |
| | | 182A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 136.2kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 43.8uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±1600Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 550.0mm(W)* 907.64mm(H)*841.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 237kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

- *2. This specification was tested under test conditions with an output voltage of $\geq 30V$.
- *3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.
- *7. Power factor of 0.99 at 50% of rated power and above at nominal input.
- *8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66168C-1600-560

| Parameter | | IT66168C-1600-560 | |
|----------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -560A~560A |
| | | 2-channel mode/Series mode | -280A~280A |
| | Power | Each channel | -84kW~84kW |
| | | Total | -168kW~168kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.286Ω |
| | | Parallel mode | 0~0.143Ω |
| | | Series mode | 0~0.572Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.017~7500Ω |
| Parallel mode | | 0.009~7500Ω | |
| Series mode | | 0.033~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |

| | | | |
|--|--|--|-----------------------------|
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.13\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.026\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.13\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Rise Time (full current) *5 | Current | $\leq 350us$ | |
| Fall Time (full current) *5 | Current | $\leq 350us$ | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | $\leq 200us$ | |
| AC Input | Input voltage *6 | Three phase + PE | 84 kW Max. @180-264V-Input |
| | | | 168 kW Max. @342-528V-Input |
| | Maximum Input Current | 292A(per phase)@200Vac, 3 ϕ input | |
| | | 307A(per phase)@380Vac, 3 ϕ input | |
| | | 243A(per phase)@480Vac, 3 ϕ input | |
| Maximum Input Apparent Power | 181.5kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | $\leq 0.005\%+0.005\%FS$ | |
| | Current | $\leq 0.01\%+0.01\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.005\%+0.005\%FS$ | |
| | Current | $\leq 0.01\%+0.01\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.005\%+0.005\%FS$ | |
| | Current | $\leq 0.01\%+0.01\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.005\%+0.005\%FS$ | |
| | Current | $\leq 0.01\%+0.01\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 58.4uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 1600Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50 $^{\circ}C$ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 600.0mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 346kg | | |

- *1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.
- *2. This specification was tested under test conditions with an output voltage of $\geq 30V$.
- *3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.
- *7. Power factor of 0.99 at 50% of rated power and above at nominal input.
- *8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66210C-1600-700

| Parameter | | IT66210C-1600-700 | |
|----------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -700A~700A |
| | | 2-channel mode/Series mode | -350A~350A |
| | Power | Each channel | -105kW~105kW |
| | | Total | -210kW~210kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.229Ω |
| | | Parallel mode | 0~0.115Ω |
| | | Series mode | 0~0.458Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.014~7500Ω |
| Parallel mode | | 0.007~7500Ω | |
| Series mode | | 0.027~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\%+0.02\%FS$ | |

| | | | |
|--|--|--------------------------|---|
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.14\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.028\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.14\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^\circ C$ | |
| | Current | $\leq 30PPM/^\circ C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^\circ C$ | |
| | Current | $\leq 30PPM/^\circ C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Rise Time (full current) *5 | Current | $\leq 500us$ | |
| Fall Time (full current) *5 | Current | $\leq 500us$ | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | $\leq 1ms$ | |
| AC Input | Input voltage *6 | Three phase + PE | 105 kW Max. @180-264V-Input 210 kW Max. @342-528V-Input |
| | | Maximum Input Current | 364A(per phase) @200Vac, 3 ϕ input 383A(per phase) @380Vac, 3 ϕ input 304A(per phase) @480Vac, 3 ϕ input |
| | Maximum Input Apparent Power | 226.9kVA | |
| | Frequency | 47Hz~63Hz | |
| | Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 73uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^\circ C \sim 70^\circ C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 1600Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | $0 \sim 50^\circ C$ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |

| Cooling | Air |
|----------------|--|
| Dimension (mm) | 600.0mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) |
| Weight(net) | 397kg |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66252C-1600-840

| Parameter | | IT66252C-1600-840 | |
|------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -840A~840A |
| | | 2-channel mode/Series mode | -420A~420A |
| | Power | Each channel | -126kW~126kW |
| | | Total | -252kW~252kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.191Ω |
| | | Parallel mode | 0~0.096Ω |
| | | Series mode | 0~0.381Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.011~7500Ω |
| Parallel mode | | 0.006~7500Ω | |
| Series mode | | 0.022~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |

| | | | |
|--|--|------------------------------------|------------------------------|
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | | | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.15%FS |
| | Vrms | 20Hz-20MHz | ≤0.03%FS |
| | Irms | 20Hz-300KHz | ≤0.15%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 126 kW Max. @ 180-264V-Input |
| | | | 252 kW Max. @ 342-528V-Input |
| | Maximum Input Current | 437A(per phase) @ 200Vac, 3ø input | |
| | | 460A(per phase) @ 380Vac, 3ø input | |
| | | 364A(per phase) @ 480Vac, 3ø input | |
| | Maximum Input Apparent Power | 272.3kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 87.6uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±1600Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |

| | | |
|------------------------|---|--------------|
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 447kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66294C-1600-980

| Parameter | | IT66294C-1600-980 | |
|-----------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -980A~980A |
| | | 2-channel mode/Series mode | -490A~490A |
| | Power | Each channel | -147kW~147kW |
| | | Total | -294kW~294kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.164Ω |
| | | Parallel mode | 0~0.082Ω |
| | | Series mode | 0~0.327Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.01~7500Ω |
| Parallel mode | | 0.005~7500Ω | |
| Series mode | | 0.019~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |

| | | | |
|---|---|--|-----------------------------|
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001 Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.16\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.032\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.16\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Rise Time (full current) *5 | Current | $\leq 500us$ | |
| Fall Time (full current) *5 | Current | $\leq 500us$ | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | $\leq 1ms$ | |
| AC Input | Input voltage *6 | Three phase + PE | 147 kW Max. @180-264V-Input |
| | | | 294 kW Max. @342-528V-Input |
| | Maximum Input Current | 510A(per phase)@200Vac, 3 ϕ input | |
| | | 537A(per phase)@380Vac, 3 ϕ input | |
| | | 425A(per phase)@480Vac, 3 ϕ input | |
| | Maximum Input Apparent Power | 317.7kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 102.2uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |

| | | |
|-----------------------------------|---|--------------|
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±1600Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 497kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66336C-1600-1120

| Parameter | | IT66336C-1600-1120 | |
|-------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -1120A~1120A |
| | | 2-channel mode/Series mode | -560A~560A |
| | Power | Each channel | -168kW~168kW |
| | | Total | -336kW~336kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.143Ω |
| | | Parallel mode | 0~0.072Ω |
| | | Series mode | 0~0.286Ω |

| | | | |
|--|----------------------------------|-----------------------|--|
| | Load resistance (CC priority) | 2-channel mode | 0.009~7500Ω |
| | | Parallel mode | 0.005~7500Ω |
| | | Series mode | 0.017~7500Ω |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.17%FS |
| | Vrms | 20Hz-20MHz | ≤0.034%FS |
| | Irms | 20Hz-300KHz | ≤0.17%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 168 kW Max. @180-264V-Input 336 kW Max. @342-528V-Input |
| | | Maximum Input Current | 583A(per phase)@200Vac, 3ø input 613A(per phase)@380Vac, 3ø input 486A(per phase)@480Vac, 3ø input |
| | Maximum Input Apparent Power | 363kVA | |
| | Frequency | 47Hz~63Hz | |
| | Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 116.8uF/CH | |

| | | |
|-----------------------------------|---|--------------|
| Min. operating voltage | ≤0.5%FS | |
| Remote Sense Voltage | 1%FS | |
| Command Response Time | 1ms | |
| Storage Temperature | -10°C~70°C | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±1600Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 583kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66378C-1600-1260

| Parameter | | | IT66378C-1600-1260 |
|-------------|---------|------------------------------|--------------------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel mode/Parallel mode | 0~800V |
| | Current | Parallel mode | -1260A~1260A |
| | | 2-channel mode/Series mode | -630A~630A |
| | Power | Each channel | -189kW~189kW |

| | | | |
|---|------------------------------------|----------------------------------|-----------------------------|
| | Resistance in series (CV priority) | Total | -378kW~378kW |
| | | 2-channel mode | 0~0.127Ω |
| | | Parallel mode | 0~0.064Ω |
| | Load resistance (CC priority) | Series mode | 0~0.254Ω |
| | | 2-channel mode | 0.008~7500Ω |
| | | Parallel mode | 0.004~7500Ω |
| | Series mode | 0.015~7500Ω | |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.18%FS |
| | Vrms | 20Hz-20MHz | ≤0.036%FS |
| | Irms | 20Hz-300KHz | ≤0.18%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 189 kW Max. @180-264V-Input |
| | | | 378 kW Max. @342-528V-Input |
| | Maximum Input Current | 655A(per phase)@200Vac, 3ø input | |
| | | 690A(per phase)@380Vac, 3ø input | |
| | | 546A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 408.4kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |

| | | |
|-----------------------------------|---|--------------|
| Efficiency | Full current and full power | ~94.5% |
| | Full voltage and full power | ~95% |
| Output Port Capacitance | 2-channel mode | 131.4uF/CH |
| Min. operating voltage | ≤0.5%FS | |
| Remote Sense Voltage | 1%FS | |
| Command Response Time | 1ms | |
| Storage Temperature | -10°C~70°C | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±1600Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 633kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66420C-1600-1400

| Parameter | | IT66420C-1600-1400 | |
|-------------|---------|--------------------|---------|
| Rated value | Voltage | Series mode | 0~1600V |
| | | 2-channel | 0~800V |

| | | | |
|---|------------------------------------|----------------------------------|-----------------------------|
| | Current | mode/Parallel mode | |
| | | Parallel mode | -1400A~1400A |
| | Power | 2-channel mode/Series mode | -700A~700A |
| | | Each channel | -210kW~210kW |
| | Resistance in series (CV priority) | Total | -420kW~420kW |
| | | 2-channel mode | 0~0.115Ω |
| | | Parallel mode | 0~0.058Ω |
| | Load resistance (CC priority) | Series mode | 0~0.229Ω |
| | | 2-channel mode | 0.007~7500Ω |
| Parallel mode | | 0.004~7500Ω | |
| Line Regulation | Series mode | 0.014~7500Ω | |
| | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.19%FS |
| | Vrms | 20Hz-20MHz | ≤0.038%FS |
| | Irms | 20Hz-300KHz | ≤0.19%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 210 kW Max. @180-264V-Input |
| | | | 420 kW Max. @342-528V-Input |
| | Maximum Input Current | 728A(per phase)@200Vac, 3ø input | |
| | | 766A(per phase)@380Vac, 3ø input | |
| | | 607A(per phase)@480Vac, 3ø input | |
| Maximum Input Apparent Power | 453.8kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |

| | | | |
|-----------------------------------|---|--------------------------|--|
| Readback Stability-30min | Current | $\leq 0.02\% + 0.02\%FS$ | |
| | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| | | | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 146uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 1600Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | $0 \sim 50^{\circ}C$ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 683kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/Rset - \Delta I) - Rset$. where V is the external voltage, $Rset$ is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds $40^{\circ}C$, the rated current and power decrease by 3% for every $1^{\circ}C$ increase. When the cabinet temperature exceeds $30^{\circ}C$, they decrease by 2% for every $1^{\circ}C$ increase. Both are applicable up to a maximum of $50^{\circ}C$.

IT6642C-2250-100

| Parameter | | IT6642C-2250-100 | |
|---|------------------------------------|---------------------------------|----------------------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -100A~100A |
| | | 2-channel mode/Series mode | -50A~50A |
| | Power | Each channel | -21kW~21kW |
| | | Total | -42kW~42kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~2.4Ω |
| | | Parallel mode | 0~1.2Ω |
| | | Series mode | 0~4.5Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.092~7500Ω |
| Parallel mode | | 0.046~7500Ω | |
| Series mode | | 0.183~7500Ω | |
| Line Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.01%FS | |
| Load Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.015%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.1%FS |
| | Vrms | 20Hz-20MHz | ≤0.02%FS |
| | Irms | 20Hz-300KHz | ≤0.1%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤1ms | |
| Rise Time (full load) *4 | Voltage | ≤1ms | |
| Fall Time (no load) *3 | Voltage | ≤1ms | |
| Fall Time (full load) *4 | Voltage | ≤1ms | |
| Rise Time (full current) *5 | Current | ≤350us | |
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 21 kW Max. @180-264V-Input |
| | | | 42 kW Max. @342-528V-Input |
| | Maximum Input Current | 73A(per phase)@200Vac, 3ø input | |
| | | 77A(per phase)@380Vac, 3ø input | |
| 61A(per phase)@480Vac, 3ø input | | | |
| Maximum Input | 45.4kVA | | |

| | | | |
|-----------------------------------|---|------------------|--|
| | Apparent Power | | |
| | Frequency | 47Hz~63Hz | |
| | Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 14.6uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±2250Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 483mm(W)* 151.3mm(H)* 831.6mm(D) | | |
| Weight(net) | (48.5±1) kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for

every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT6684C-2250-200

| Parameter | | IT6684C-2250-200 | |
|---|------------------------------------|------------------------------|----------------------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -200A~200A |
| | | 2-channel mode/Series mode | -100A~100A |
| | Power | Each channel | -42kW~42kW |
| | | Total | -84kW~84kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~1.2Ω |
| | | Parallel mode | 0~0.6Ω |
| | | Series mode | 0~2.25Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.046~7500Ω |
| Parallel mode | | 0.023~7500Ω | |
| Series mode | | 0.092~7500Ω | |
| Line Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.01%FS | |
| Load Regulation | Voltage | ≤0.005%FS | |
| | Current | ≤0.015%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.01%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | V _{pp} | 20Hz-20MHz | ≤0.11%FS |
| | V _{rms} | 20Hz-20MHz | ≤0.022%FS |
| | I _{rms} | 20Hz-300KHz | ≤0.11%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤1ms | |
| Rise Time (full load) *4 | Voltage | ≤1ms | |
| Fall Time (no load) *3 | Voltage | ≤1ms | |
| Fall Time (full load) *4 | Voltage | ≤1ms | |
| Rise Time (full current) *5 | Current | ≤350us | |
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 42 kW Max. @180-264V-Input |
| | | | 84 kW Max. @342-528V-Input |

| | | |
|-----------------------------------|------------------------------|--|
| | Maximum Input Current | 146A(per phase)@200Vac, 3 ϕ input |
| | | 154A(per phase)@380Vac, 3 ϕ input |
| | | 122A(per phase)@480Vac, 3 ϕ input |
| | Maximum Input Apparent Power | 90.8kVA |
| | Frequency | 47Hz~63Hz |
| | Power Factor *7 | 0.99 |
| Setup Stability-30min | Voltage | $\leq 0.005\% + 0.005\%FS$ |
| | Current | $\leq 0.01\% + 0.01\%FS$ |
| Setup Stability-8h | Voltage | $\leq 0.005\% + 0.005\%FS$ |
| | Current | $\leq 0.01\% + 0.01\%FS$ |
| Readback Stability-30min | Voltage | $\leq 0.005\% + 0.005\%FS$ |
| | Current | $\leq 0.01\% + 0.01\%FS$ |
| Readback Stability-8h | Voltage | $\leq 0.005\% + 0.005\%FS$ |
| | Current | $\leq 0.01\% + 0.01\%FS$ |
| Efficiency | Full current and full power | ~94.5% |
| | Full voltage and full power | ~95% |
| Output Port Capacitance | 2-channel mode | 29.2uF/CH |
| Min. operating voltage | | $\leq 0.5\%FS$ |
| Remote Sense Voltage | | 1%FS |
| Command Response Time | | 1ms |
| Storage Temperature | | -10 $^{\circ}C$ ~70 $^{\circ}C$ |
| Protective Function | | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection |
| Standard Interface | | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards |
| Maximum Working Isolation Voltage | | $\pm 2250Vdc$ |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | | 0~50 $^{\circ}C$ |
| IP | | IP20 |
| Safety Standard | | IEC 61010 |
| Cooling | | Air |
| Dimension (mm) | | 550.0mm(W)* 907.64mm(H)*841.1mm(1008.1mm including protective cover)(D) |
| Weight(net) | | 186kg |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/Rset - \Delta I) - Rset$. where V is the external voltage, $Rset$ is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models,

the standard AC input voltage only supports 380VAC \pm 10%, such as the need for 480VAC \pm 10% voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66126C-2250-300

| Parameter | | IT66126C-2250-300 | |
|-----------------------------------|------------------------------------|------------------------------|------------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -300A~300A |
| | | 2-channel mode/Series mode | -150A~150A |
| | Power | Each channel | -63kW~63kW |
| | | Total | -126kW~126kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.8Ω |
| | | Parallel mode | 0~0.4Ω |
| | | Series mode | 0~1.5Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.031~7500Ω |
| Parallel mode | | 0.016~7500Ω | |
| Series mode | | 0.061~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\%+0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\%+0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.12\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.024\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.12\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^\circ C$ | |
| | Current | $\leq 30PPM/^\circ C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^\circ C$ | |
| | Current | $\leq 30PPM/^\circ C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 1ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 1ms$ | |
| Rise Time (full current) *5 | Current | $\leq 350us$ | |
| Fall Time (full current) *5 | Current | $\leq 350us$ | |

| | | | |
|--|---|----------------------------------|---|
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 63 kW Max. @180-264V-Input 126 kW Max. @342-528V-Input |
| | Maximum Input Current | 219A(per phase)@200Vac, 3ø input | |
| | | 230A(per phase)@380Vac, 3ø input | |
| | | 182A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 136.2kVA | |
| | Frequency | 47Hz~63Hz | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 43.8uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±2250Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 550.0mm(W)* 907.64mm(H)*841.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 237kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-

impedance DC Bi-directional source, when the output current makes a step change from $-100\%FS$ to $+100\%FS$ (or $+100\%FS$ to $-100\%FS$), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports $380VAC \pm 10\%$, such as the need for $480VAC \pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds $40^{\circ}C$, the rated current and power decrease by 3% for every $1^{\circ}C$ increase. When the cabinet temperature exceeds $30^{\circ}C$, they decrease by 2% for every $1^{\circ}C$ increase. Both are applicable up to a maximum of $50^{\circ}C$.

IT66168C-2250-400

| Parameter | | IT66168C-2250-400 | |
|-----------------------------------|------------------------------------|------------------------------|------------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -400A~400A |
| | | 2-channel mode/Series mode | -200A~200A |
| | Power | Each channel | -84kW~84kW |
| | | Total | -168kW~168kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.6Ω |
| | | Parallel mode | 0~0.3Ω |
| | | Series mode | 0~1.125Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.023~7500Ω |
| Parallel mode | | 0.012~7500Ω | |
| Series mode | | 0.046~7500Ω | |
| Line Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.01\%FS$ | |
| Load Regulation | Voltage | $\leq 0.005\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.001A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.01\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.13\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.026\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.13\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 1ms$ | |

| | | | |
|--|--|----------------------------------|---|
| Rise Time (full load) *4 | Voltage | ≤1ms | |
| Fall Time (no load) *3 | Voltage | ≤1ms | |
| Fall Time (full load) *4 | Voltage | ≤1ms | |
| Rise Time (full current) *5 | Current | ≤350us | |
| Fall Time (full current) *5 | Current | ≤350us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤200us | |
| AC Input | Input voltage *6 | Three phase + PE | 84 kW Max. @180-264V-Input 168 kW Max. @342-528V-Input |
| | Maximum Input Current | 292A(per phase)@200Vac, 3ø input | |
| | | 307A(per phase)@380Vac, 3ø input | |
| | | 243A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 181.5kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Setup Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-30min | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Readback Stability-8h | Voltage | ≤0.005%+0.005%FS | |
| | Current | ≤0.01%+0.01%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 58.4uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±2250Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 600.0mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 346kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/Rset - \Delta I) - Rset$. where V is the external voltage, $Rset$ is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC \pm 10%, such as the need for 480VAC \pm 10% voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66210C-2250-500

| Parameter | | IT66210C-2250-500 | |
|----------------------|------------------------------------|------------------------------|------------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -500A~500A |
| | | 2-channel mode/Series mode | -250A~250A |
| | Power | Each channel | -105kW~105kW |
| | | Total | -210kW~210kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.48Ω |
| | | Parallel mode | 0~0.24Ω |
| | | Series mode | 0~0.9Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.019~7500Ω |
| Parallel mode | | 0.01~7500Ω | |
| Series mode | | 0.037~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\%+0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\%+0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.14\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.028\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.14\%FS$ |

| | | | |
|--|--|----------------------------------|--|
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 105 kW Max. @180-264V-Input 210 kW Max. @342-528V-Input |
| | Maximum Input Current | 364A(per phase)@200Vac, 3ø input | |
| | | 383A(per phase)@380Vac, 3ø input | |
| | | 304A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 226.9kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 73uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±2250Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 600.0mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 397kg | | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

- *2. This specification was tested under test conditions with an output voltage of $\geq 30V$.
- *3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.
- *7. Power factor of 0.99 at 50% of rated power and above at nominal input.
- *8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66252C-2250-600

| Parameter | | IT66252C-2250-600 | |
|----------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -600A~600A |
| | | 2-channel mode/Series mode | -300A~300A |
| | Power | Each channel | -126kW~126kW |
| | | Total | -252kW~252kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.4Ω |
| | | Parallel mode | 0~0.2Ω |
| | | Series mode | 0~0.75Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.016~7500Ω |
| Parallel mode | | 0.008~7500Ω | |
| Series mode | | 0.031~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\%+0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\%+0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |

| | | | |
|---|---|--------------------------|--|
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.15\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.03\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.15\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Rise Time (full current) *5 | Current | $\leq 500us$ | |
| Fall Time (full current) *5 | Current | $\leq 500us$ | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | $\leq 1ms$ | |
| AC Input | Input voltage *6 | Three phase + PE | 126 kW Max. @180-264V-Input 252 kW Max. @342-528V-Input |
| | | Maximum Input Current | 437A(per phase)@200Vac, 3ø input 460A(per phase)@380Vac, 3ø input 364A(per phase)@480Vac, 3ø input |
| | Maximum Input Apparent Power | 272.3kVA | |
| | Frequency | 47Hz~63Hz | |
| | Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | $\leq 0.01\%+0.01\%FS$ | |
| | Current | $\leq 0.02\%+0.02\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.01\%+0.01\%FS$ | |
| | Current | $\leq 0.02\%+0.02\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.01\%+0.01\%FS$ | |
| | Current | $\leq 0.02\%+0.02\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.01\%+0.01\%FS$ | |
| | Current | $\leq 0.02\%+0.02\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 87.6uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 2250Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | 0~50°C | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |
| Cooling | Air | | |
| Dimension (mm) | 600.00mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) | | |
| Weight(net) | 447kg | | |

- *1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.
- *2. This specification was tested under test conditions with an output voltage of $\geq 30V$.
- *3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.
- *6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.
- *7. Power factor of 0.99 at 50% of rated power and above at nominal input.
- *8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66294C-2250-700

| Parameter | | IT66294C-2250-700 | |
|----------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -700A~700A |
| | | 2-channel mode/Series mode | -350A~350A |
| | Power | Each channel | -147kW~147kW |
| | | Total | -294kW~294kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.343Ω |
| | | Parallel mode | 0~0.172Ω |
| | | Series mode | 0~0.643Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.014~7500Ω |
| Parallel mode | | 0.007~7500Ω | |
| Series mode | | 0.027~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\%+0.02\%FS$ | |

| | | | |
|--|--|--|--|
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.16\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.032\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.16\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Rise Time (full current) *5 | Current | $\leq 500us$ | |
| Fall Time (full current) *5 | Current | $\leq 500us$ | |
| Transient Response Time(change from 40% to 90% of rated current) | Voltage | $\leq 1ms$ | |
| AC Input | Input voltage *6 | Three phase + PE | 147 kW Max. @180-264V-Input 294 kW Max. @342-528V-Input |
| | Maximum Input Current | 510A(per phase)@200Vac, 3 ϕ input | |
| | | 537A(per phase)@380Vac, 3 ϕ input | |
| | | 425A(per phase)@480Vac, 3 ϕ input | |
| | Maximum Input Apparent Power | 317.7kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 102.2uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | $\pm 2250Vdc$ | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |
| | Input to Output | 3375Vdc/1min | |
| | Output to Ground | 3375Vdc/1min | |
| Working Temperature *8 | $0 \sim 50^{\circ}C$ | | |
| IP | IP20 | | |
| Safety Standard | IEC 61010 | | |

| Cooling | Air |
|----------------|---|
| Dimension (mm) | 600.00mm(W)* 1441.41mm(H)*840.1mm(1008.1mm including protective cover)(D) |
| Weight(net) | 497kg |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66336C-2250-800

| Parameter | | IT66336C-2250-800 | |
|------------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -800A~800A |
| | | 2-channel mode/Series mode | -400A~400A |
| | Power | Each channel | -168kW~168kW |
| | | Total | -336kW~336kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.3Ω |
| | | Parallel mode | 0~0.15Ω |
| | | Series mode | 0~0.563Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.012~7500Ω |
| Parallel mode | | 0.006~7500Ω | |
| Series mode | | 0.023~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |

| | | | |
|--|--|----------------------------------|-----------------------------|
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | | | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.17%FS |
| | Vrms | 20Hz-20MHz | ≤0.034%FS |
| | Irms | 20Hz-300KHz | ≤0.17%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 168 kW Max. @180-264V-Input |
| | | | 336 kW Max. @342-528V-Input |
| | Maximum Input Current | 583A(per phase)@200Vac, 3ø input | |
| | | 613A(per phase)@380Vac, 3ø input | |
| | | 486A(per phase)@480Vac, 3ø input | |
| | Maximum Input Apparent Power | 363kVA | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 116.8uF/CH | |
| Min. operating voltage | ≤0.5%FS | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | -10°C~70°C | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | | |
| Maximum Working Isolation Voltage | ±2250Vdc | | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min | |

| | | |
|------------------------|---|--------------|
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 583kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66378C-2250-900

| Parameter | | IT66378C-2250-900 | |
|-----------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -900A~900A |
| | | 2-channel mode/Series mode | -450A~450A |
| | Power | Each channel | -189kW~189kW |
| | | Total | -378kW~378kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.267Ω |
| | | Parallel mode | 0~0.134Ω |
| | | Series mode | 0~0.5Ω |
| | Load resistance (CC priority) | 2-channel mode | 0.011~7500Ω |
| Parallel mode | | 0.006~7500Ω | |
| Series mode | | 0.021~7500Ω | |
| Line Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.015\%FS$ | |

| | | | |
|---|---|--|-----------------------------|
| Load Regulation | Voltage | $\leq 0.01\%FS$ | |
| | Current | $\leq 0.02\%FS$ | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001 Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | $\leq 0.02\% + 0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Read Back Accuracy | Voltage | $\leq 0.02\% + 0.02\%FS$ | |
| | Current | $\leq 0.03\% + 0.03\%FS$ | |
| | Power | $\leq 0.05\% + 0.15\%FS$ | |
| | Resistance *1 | $\leq 0.5\%$ | |
| Ripple *2 | Vpp | 20Hz-20MHz | $\leq 0.18\%FS$ |
| | Vrms | 20Hz-20MHz | $\leq 0.036\%FS$ |
| | Irms | 20Hz-300KHz | $\leq 0.18\%FS$ |
| Setup Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Read Back Temperature Coefficient | Voltage | $\leq 15PPM/^{\circ}C$ | |
| | Current | $\leq 30PPM/^{\circ}C$ | |
| Rise Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Rise Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Fall Time (no load) *3 | Voltage | $\leq 2ms$ | |
| Fall Time (full load) *4 | Voltage | $\leq 2ms$ | |
| Rise Time (full current) *5 | Current | $\leq 500us$ | |
| Fall Time (full current) *5 | Current | $\leq 500us$ | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | $\leq 1ms$ | |
| AC Input | Input voltage *6 | Three phase + PE | 189 kW Max. @180-264V-Input |
| | | | 378 kW Max. @342-528V-Input |
| | Maximum Input Current | 655A(per phase)@200Vac, 3 ϕ input | |
| | | 690A(per phase)@380Vac, 3 ϕ input | |
| | | 546A(per phase)@480Vac, 3 ϕ input | |
| Maximum Input Apparent Power | 408.4kVA | | |
| Frequency | 47Hz~63Hz | | |
| Power Factor *7 | 0.99 | | |
| Setup Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Setup Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-30min | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Readback Stability-8h | Voltage | $\leq 0.01\% + 0.01\%FS$ | |
| | Current | $\leq 0.02\% + 0.02\%FS$ | |
| Efficiency | Full current and full power | $\sim 94.5\%$ | |
| | Full voltage and full power | $\sim 95\%$ | |
| Output Port Capacitance | 2-channel mode | 131.4uF/CH | |
| Min. operating voltage | $\leq 0.5\%FS$ | | |
| Remote Sense Voltage | 1%FS | | |
| Command Response Time | 1ms | | |
| Storage Temperature | $-10^{\circ}C \sim 70^{\circ}C$ | | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | | |

| | | |
|-----------------------------------|--|--------------|
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232), fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±2250Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 633kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

IT66420C-2250-1000

| Parameter | | IT66420C-2250-1000 | |
|-------------|------------------------------------|------------------------------|--------------|
| Rated value | Voltage | Series mode | 0~2250V |
| | | 2-channel mode/Parallel mode | 0~1200V |
| | Current | Parallel mode | -1000A~1000A |
| | | 2-channel mode/Series mode | -500A~500A |
| | Power | Each channel | -210kW~210kW |
| | | Total | -420kW~420kW |
| | Resistance in series (CV priority) | 2-channel mode | 0~0.24Ω |
| | | Parallel mode | 0~0.12Ω |
| | | Series mode | 0~0.45Ω |

| | | | |
|---|-------------------------------|-----------------------|--|
| | Load resistance (CC priority) | 2-channel mode | 0.01 ~ 7500Ω |
| | | Parallel mode | 0.005 ~ 7500Ω |
| | | Series mode | 0.019 ~ 7500Ω |
| Line Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.015%FS | |
| Load Regulation | Voltage | ≤0.01%FS | |
| | Current | ≤0.02%FS | |
| Setup Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| | Resistance | 0.001Ω | |
| Read Back Resolution | Voltage | 0.001V | |
| | Current | 0.01A | |
| | Power | 0.001kW | |
| Setup Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Read Back Accuracy | Voltage | ≤0.02%+0.02%FS | |
| | Current | ≤0.03% + 0.03%FS | |
| | Power | ≤0.05% + 0.15%FS | |
| | Resistance *1 | ≤0.5% | |
| Ripple *2 | Vpp | 20Hz-20MHz | ≤0.19%FS |
| | Vrms | 20Hz-20MHz | ≤0.038%FS |
| | Irms | 20Hz-300KHz | ≤0.19%FS |
| Setup Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Read Back Temperature Coefficient | Voltage | ≤15PPM/°C | |
| | Current | ≤30PPM/°C | |
| Rise Time (no load) *3 | Voltage | ≤2ms | |
| Rise Time (full load) *4 | Voltage | ≤2ms | |
| Fall Time (no load) *3 | Voltage | ≤2ms | |
| Fall Time (full load) *4 | Voltage | ≤2ms | |
| Rise Time (full current) *5 | Current | ≤500us | |
| Fall Time (full current) *5 | Current | ≤500us | |
| Transient Response Time (change from 40% to 90% of rated current) | Voltage | ≤1ms | |
| AC Input | Input voltage *6 | Three phase + PE | 210 kW Max. @180-264V-Input 420 kW Max. @342-528V-Input |
| | | Maximum Input Current | 728A(per phase)@200Vac, 3ø input 766A(per phase)@380Vac, 3ø input 607A(per phase)@480Vac, 3ø input |
| | Maximum Input Apparent Power | 453.8kVA | |
| | Frequency | 47Hz~63Hz | |
| | Power Factor *7 | 0.99 | |
| Setup Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Setup Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-30min | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Readback Stability-8h | Voltage | ≤0.01%+0.01%FS | |
| | Current | ≤0.02%+0.02%FS | |
| Efficiency | Full current and full power | ~94.5% | |
| | Full voltage and full power | ~95% | |
| Output Port Capacitance | 2-channel mode | 146uF/CH | |

| | | |
|-----------------------------------|---|--------------|
| Min. operating voltage | ≤0.5%FS | |
| Remote Sense Voltage | 1%FS | |
| Command Response Time | 1ms | |
| Storage Temperature | -10°C~70°C | |
| Protective Function | OVP, OCP, OPP, UVP, UCP, OTP, Vsense protection | |
| Standard Interface | Standard: USB, CAN, LAN, Digital IO Optional: GPIB, Analog/RS232, fiber optic socket, EtherCAT card, Relay cards | |
| Maximum Working Isolation Voltage | ±2250Vdc | |
| Withstand Voltage | Input to Ground | 3000Vdc/1min |
| | Input to Output | 3375Vdc/1min |
| | Output to Ground | 3375Vdc/1min |
| Working Temperature *8 | 0~50°C | |
| IP | IP20 | |
| Safety Standard | IEC 61010 | |
| Cooling | Air | |
| Dimension (mm) | 600.00mm(W)* 1885.91mm(H)*840.1mm(1008.1mm including protective cover)(D) | |
| Weight(net) | 683kg | |

*1. This accuracy specification applies to output power in the range of 10% to 100%. When the output power is low, the resistance deviation (ΔR) can be approximated by: $\Delta R \approx V / (V/R_{set} - \Delta I) - R_{set}$. where V is the external voltage, R_{set} is the set resistance value, and ΔI is the theoretical current deviation of the IT6600.

*2. This specification was tested under test conditions with an output voltage of $\geq 30V$.

*3. No-load voltage rise/fall time: With the instrument operating in CV mode and no load connected, when the output voltage makes a step change from 10%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*4. Full-load voltage rise/fall time: With the instrument operating in CV mode and with full load (constant-current load), when the output voltage makes a step change from 0.1%FS to 100%FS (or 100%FS to 0.1%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*5. Full-current rise/fall time: With the instrument operating in CC mode and connected to a low-impedance DC Bi-directional source, when the output current makes a step change from -100%FS to +100%FS (or +100%FS to -100%FS), the time for the output to transition from 10% to 90% of the step amplitude.

*6. Multi-master cabinet, that is, optional emergency stop module (including AC contactor) models, the standard AC input voltage only supports 380VAC $\pm 10\%$, such as the need for 480VAC $\pm 10\%$ voltage need to be customized.

*7. Power factor of 0.99 at 50% of rated power and above at nominal input.

*8. When the unit temperature exceeds 40°C, the rated current and power decrease by 3% for every 1°C increase. When the cabinet temperature exceeds 30°C, they decrease by 2% for every 1°C increase. Both are applicable up to a maximum of 50°C.

All the above parameters are subject to change without prior notice from ITECH.

Chapter8 Remote Control

This series power supply comes standard with three communication interfaces: USB, LAN and CAN, and supports two optional communication interfaces: GPIB, RS232. You can choose one of them to communicate with your computer.

When you use the remote interface to send SCPI instructions, if you use the programming commands that involve modifying the instrument settings, such as modifying the output voltage value, after completing the communication connection between the instrument and the host computer, and after the communication settings are completed, you must execute the **SYST:REM** command firstly.

8.1 USB Interface

The USB interface is located on the rear panel of the instrument. You can connect the instrument to the computer via a cable with a USB interface on both ends (USB A-type connector on one end and USB B-type connector on the other).

Operation step

The operation steps to change the USB interface type in System Menu are as follows.

1. Press the composite keys [**Shift**] + [**P-set**] (System) on the front panel to enter the system menu.
2. Select Communication ->**USB** and press [**Enter**].
3. Select **USB Type** to Device, and press [**Enter**].
4. Select the USB device class to TMC or VCP, and press [**Enter**].

8.2 LAN Interface

When the user connect PC through LAN interface, the following is required to use the LAN interface. The LAN interface complies with the LXI standard.

Connect Interface

Use the following steps to quickly connect your instrument to your LAN and configure it. Two typical LAN interface systems are described below: private LAN and site LAN.

- Connect to the private LAN

A private LAN is a network in which LAN-enabled instruments and computers are directly connected. They are typically small, with no centrally-managed resources. When connected to a computer, a standard network cable can be used to connect directly to the computer via the LAN interface.

- Connect to the site LAN

A site LAN is a local area network in which LAN-enabled instruments and computers are connected to the network through routers, hubs, and/or switches. They are typically large, centrally-managed networks with

services such as DHCP and DNS servers. When connected to a computer, a network cable can be used to connect to the router, and the computer is also connected to the router.



Note

- When using one crossover cable to connect PC directly, the gateway address of the instrument should be consistent with that of the PC, and the IP address should be at the same network segment with the PC's IP address.
- When the instrument and computer are connected to the router, an independent IP address must be assigned for the instrument.

Configure LAN Interface Information

The configurable parameters of the IT6600 series power supply are described as follows.

LAN Config:

- Mode: IP Address setting method, user can select automatically configure the address of the instrument (DHCP) or manually.
- IP: This value is the Internet Protocol (IP) address of the instrument. An IP address is required for all IP and TCP/IP communications with the instrument. An IP Address consists of 4 decimal numbers separated by periods. Each decimal number ranges from 0 through 255 with no leading zeros (for example, 169.254.2.20).
- Mask: This value is used to enable the instrument to determine if a client IP address is on the same local subnet. The same numbering notation applies as for the IP Address. When a client IP address is on a different subnet, all packets must be sent to the Default Gateway.
- Gateway: This value is the IP Address of the default gateway that allows the instrument to communicate with systems that are not on the local subnet, as determined by the subnet mask setting. The same numbering notation applies as for the IP Address.
- Socket Port: This value indicates the port number corresponding to the service.

How to Configure

Take manual configuration as an example. The steps are as follows:


1. Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
2. Select **Communication** and press **[Enter]**.
3. Press the Left/Right key to select **LAN** and set the mode to **Manual**.
4. Set the **IP**, **Mask** and the other parameters in turns, and press **[Enter]**.

8.2.1 Using Web Server

The instrument provides a built-in web server, allowing you to monitor it directly from your computer's web browser. To use this web server, connect the instrument and the computer via the LAN interface. Then, enter the instrument's IP address in the address bar at the top of the computer's web browser to access front panel control, including LAN configuration parameters.

The address format to be entered in the browser's address bar is: `http://192.168.200.100`.

192.168.200.100 is the default IP address. If it has been changed by the user, replace this IP with the actual configuration found in the instrument's Menu.

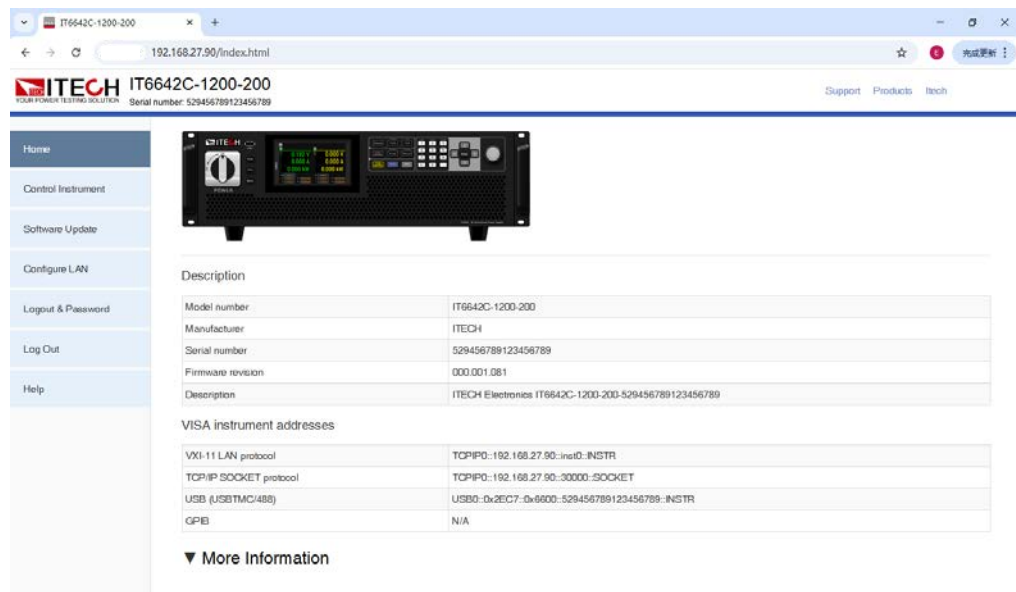

You can select different pages by clicking the buttons shown in the navigation bar on the left side of the window. The detailed descriptions are as follows.

- **Home:** The main web interface that displays the instrument model, appearance image, and key information including Description, VISA instrument addresses, and LAN details.
- **Control Instrument:** Enables the Web control to begin controlling the instrument. This page allows you to monitor and control the instrument. The initial login password is itech.
- **Software Update:** Performs a system upgrade.
Click [Click here](#), to select the system upgrade installation package (for example, IT6600-U-VXXX.itech), and then click **Update** performs the upgrade operation. After the upgrade is complete, the instrument needs to be restarted.
- **Configure LAN:** Reconfigure the LAN parameters.
- **Password:** Modify the login password for the Control Instrument and Software Update pages to control access to the Web interface.
- **Logout:** logout the Web interface.
- **Help:** Detailed instructions for using the Web features.

8.2.2 Using Telnet

The Telnet utility (as well as sockets), is another way to communicate with the instrument without using I/O libraries or drivers. In all cases, you must first establish a LAN connection from your computer to the instrument as previously described.

In an MS-DOS Command Prompt box, type “telnet hostname” where hostname is the instrument’s hostname or IP address. Press the Enter key and you should get a Telnet session box with a title indicating that you are connected to the

instrument and 23 is the instrument's telnet port. Type the SCPI commands at the prompt.

8.2.3 Using Sockets

CAUTION

- Before using this function, you need to configure **Socket Port**, and the configuration on the instrument side should be consistent with the configuration on the PC side.
- The instruments allow any combination of up to six simultaneous socket and telnet connections to be made.


ITECH instruments have SCPI socket services, which can be used to send and receive SCPI commands, queries, and query responses. All commands must be terminated with a newline for the message to be parsed. All query responses will also be terminated with a newline.

8.2.4 Using VNC

VNC (Virtual Network Computing) is a method of controlling a machine from a remote desktop. Before using VNC, make sure to connect the machine and computer using a LAN connection and configure the machine's IP address to ensure they are on the same LAN.


Using the Browser

Enter the IP address of the machine + port number in the address bar of your browser and press enter to connect to the machine. Note that the port number must be 5800. The opened page is displayed as follows:



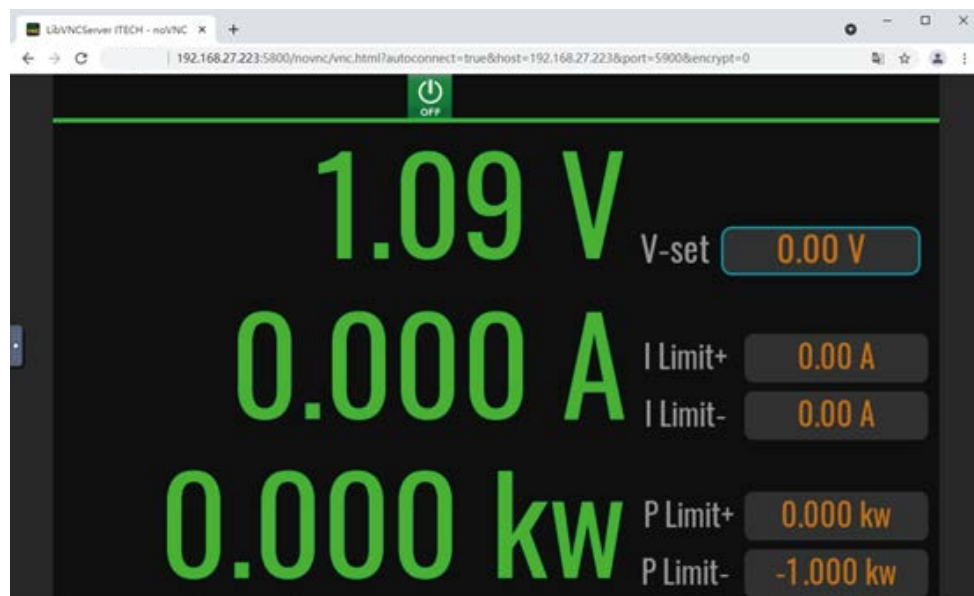


Using the VNC Client

1. Double-click the VNC client software.



2. In the software that opens, enter the IP address of the machine in the edit box and press enter to connect to access the machine.

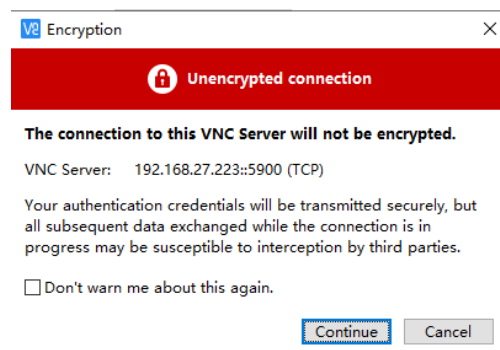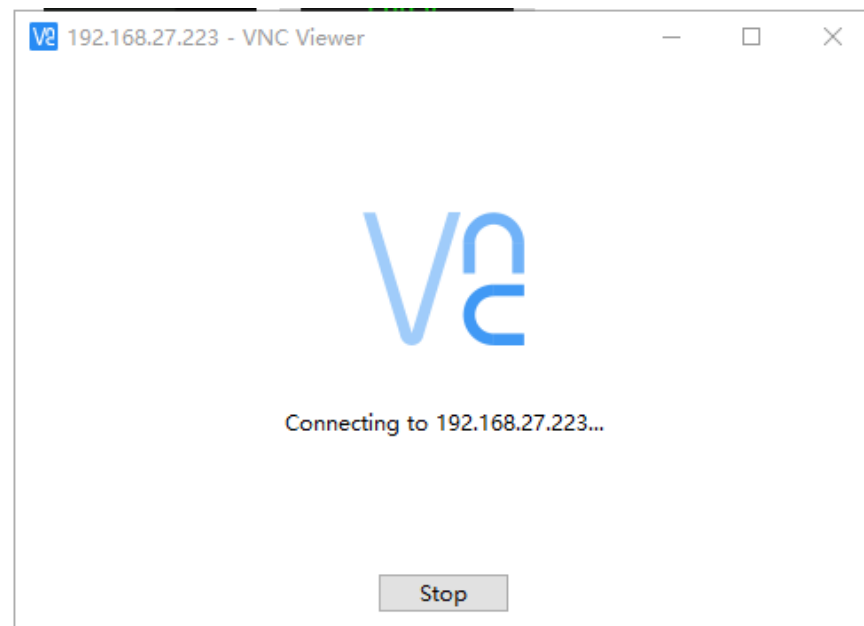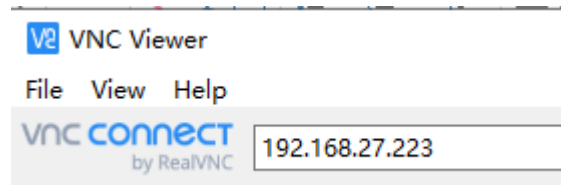

3. Click [Continue] to display the machine touch screen.



8.3 CAN Interface

The CAN interface is located on the rear panel of the instrument and is connected to the computer using a CAN communication cable. The definition of CAN pins are as follows.

| Pins | Description |
|------|-------------|
| H | CAN_H |
| L | CAN_L |

CAN Configuration

The user needs to configure the CAN interface parameters in the system menu before using the remote control. The CAN interface parameters are as follows.

| Name | Description |
|-----------|---|
| Baud rate | Select the baud rate from the following options: 5k/10k/20k/40k/50k/80k/100k/125k/200k/250k/400k/500k/600k/800k/1000k. |
| Address | Range: 0 – 127. |
| Protocol | <ul style="list-style-type: none"> ● CAN_OPEN: High-level protocol for the CAN bus. ● CAN2.0: ITECH CAN version 2.0 protocol. |


The operation steps are as follows.

1. Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
2. Select **Communication** and press **[Enter]**.
3. Select **CAN** and press **[Enter]**.
4. Set the baud rate and address, press **[Enter]**.


CAN Troubleshooting

If you meet some problems when communicating with PC by CAN interface, please check the following items:

- PC and the instrument must have the same baud rate.
 - Ensure you have used the correct communication cable (CAN_H, CAN_L). Please pay attention that some cable may not have a correct internal wiring even it is with an appropriate plug.
 - The interface cable is correctly connected (CAN_H to CAN_H, CAN_L to CAN_L).
 - If the communication signal is poor or unstable, it is recommended to connect a 120 Ω terminating resistance.
- The connection diagram of a single device is as below.

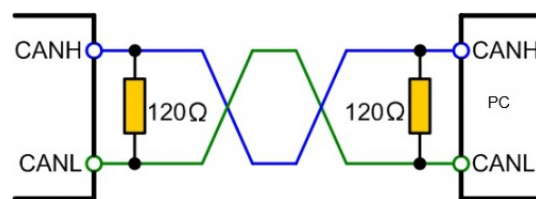

- The connection diagram of multiple devices is as below.

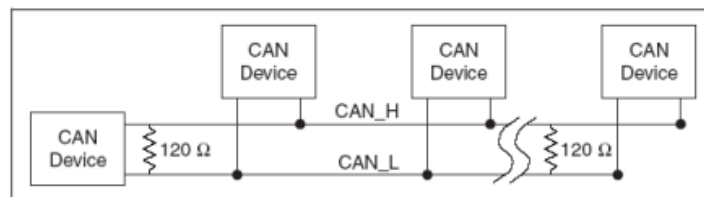

8.4 GPIB Interface (Optional)

The GPIB (IEEE-488) interface is assembled in the IT-E176 communication board. Use a GPIB cable to connect GPIB interfaces of the instrument and PC. Please ensure that the screws have been screwed down in order to have a full connection.

GPIB Configuration

Each device on the GPIB (IEEE-488) interface must have a unique whole number address between 1 and 30. Your computer's GPIB interface card address must not conflict with any instrument on the interface bus. This setting is nonvolatile; it will not be changed by *RST.

When you purchase the interface accessory and successfully insert it into the corresponding position on the rear panel of the instrument, the menu item for changing the GPIB address appears in the System menu. The specific steps are as follows:

1. Ensure that the instrument's power switch is off, that is, the instrument is in Power Off state.
2. Insert the separately purchased GPIB interface card into the card slot on the rear panel of the instrument.
3. Connect the instrument with the computer via the GPIB cable. After the connection is successful, turn on the power switch of the instrument.

4. Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
5. Select **Communication** and press **[Enter]**.
6. Select **GPIB** and press **[Enter]**.
7. Press the numeric keys to set the GPIB address and press **[Enter]**.

8.5 RS232 Interface (Optional)

The RS232 interface shares the same communication card (IT-E177) with the analog function.

RS232 Cable


Use the supplied RS232 cable (one end with a DB9 connector and the other with a flat terminal) to connect the instrument to the PC. The connection method is as follows: the flat terminal connects to the communication board (the board is inserted into the rear panel of the instrument), and the DB9 connector connects to the PC. The connection of the flat terminal is as follows:

- TXD wire (red) connects to Pin1 of the communication board.
- RXD wire (white) connects to Pin2 of the communication board.
- DGND wire (black) connects to Pin3 of the communication board.




Note

- If the PC has a DB9 interface, you can directly use the supplied RS232 cable by connecting the DB9 end to the PC.
- If the PC only has a USB interface, you will need an RS232 to USB adapter cable for the connection. This type of adapter cable requires a driver to function correctly as a COM port. Please contact the supplier of the RS232–USB adapter cable for the necessary driver.

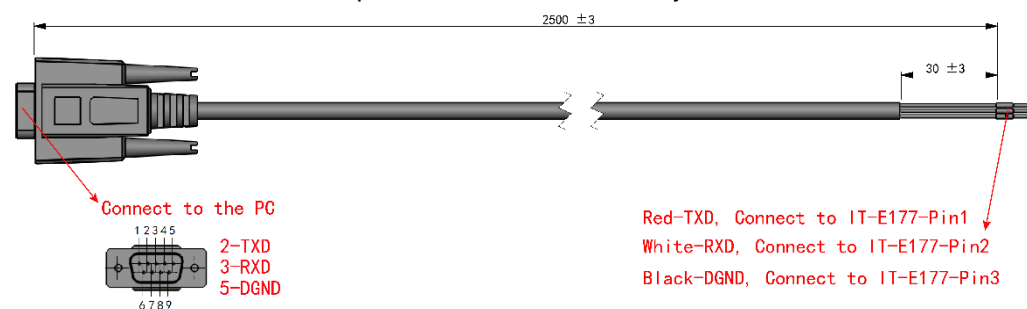

Definition of RS232 Pins

The definition of RS232 pins are as follows.

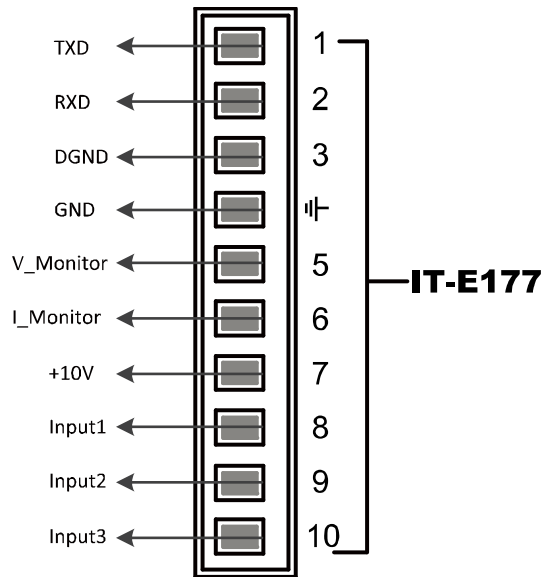

When using the RS232 interface for communication, connect the pin 1, pin 2, and pin 3 of the IT-E177 to the PC. The pin description is as follows:

| Pins | Description |
|------|--------------------|
| 1 | TXD, transmit data |
| 2 | RXD, receive data |
| 3 | DGND, ground |

RS232 Configuration

When you purchase the interface accessory and successfully insert it into the corresponding position on the rear panel of the instrument, the RS232 menu item will appear in the System menu. The specific steps are as follows:

1. Ensure that the instrument's power switch is off, that is, the instrument is in Power Off state.
2. Insert the separately purchased RS232 interface card into the card slot on the rear panel of the instrument.
3. Connect the instrument to the computer via an RS232 cable. After the connection is successful, turn on the power switch of the instrument.
4. Press the composite keys **[Shift] + [P-set]** (System) on the front panel to enter the system menu.
5. Select **Communication** and press **[Enter]**.
6. Select **RS232** and press **[Enter]**.
7. Set the relevant communication parameters in turn, and press **[Enter]**.

RS232 Troubleshooting

If you meet some problems when communicating with PC by RS232 interface, please check the following items:

- Check that whether the baud rate of the computer and instrument are the same;
- Make sure the correct cable and adapter are connected. Note that internal

wiring may not be correct even if the cable has a suitable plug;

- The cable must be connected to the correct serial ports (COM1, COM2, etc) of PC.

8.6 EtherCAT Interface (Optional)

The EtherCAT interface is assembled in the IT-E1601-black communication board. You can connect the instrument to the computer via a network cable.

EtherCAT Configuration

When you purchase the interface accessory and successfully insert it into the corresponding position on the rear panel of the instrument, the menu item for EtherCAT configuration appears in the System menu. The specific steps are as follows.

1. Ensure that the instrument's power switch is off, that is, the instrument is in Power Off state.
2. Insert the separately purchased EtherCAT interface card into the card slot on the rear panel of the instrument.
3. Connect the instrument with the computer via the network cable. After the connection is successful, turn on the power switch of the instrument.
4. Click **System** on the Menu interface to enter the system menu function page.
5. Click the **COMM** tab to enter the communication settings page.
6. Scroll up and down on the **COMM** settings interface to locate the menu item **Card Config**.

At the **Type** function, click the parameter on the right and select **ECAT** from the dropdown options.

7. After making the communication setting, to ensure normal communication, you need to restart the instrument.
8. Repeat steps 4~6 above to view the EtherCAT information.

| Display Information | Function |
|-----------------------------|--|
| Card Config | - |
| State: Init/Preop/Safeop/Op | State: Initialization/Pre-operational/Safe-operational/Operational. |
| Addr: 1001 | Slave address (this address is assigned to this slave by the EtherCAT master). |
| Alias Addr: 1 | Slave address alias. |
| HW Ver: 256 | Communication card hardware version number. |
| Soft Ver: 1 | Communication card software version number. |

Appendix

Specifications of Red and Black Test Lines

ITECH provides you with optional red and black test lines, the user can choose the company's test line for testing. For specifications of ITECH test lines and maximum current values, refer to the table below.

| Model | Description |
|-----------------|--|
| IT-E30110-AB | 1kV/10A/1m*2pcs Alligator clips-Banana plugs |
| IT-E30110-BB | 1kV/10A/1m*2pcs Banana plugs-Banana plugs |
| IT-E30110-BY | 1kV/10A/1m*2pcs Banana plugs-Y-type terminals |
| IT-E30312-YY | 500V/30A/1.2m*2pcs Y-type terminals-Y-type terminals |
| IT-E30320-YY | 500V/30A/2m*2pcs Y-type terminals-Y-type terminals |
| IT-E30615-OO | 500V/60A/1.5m*2pcs Ring terminals-Ring terminals |
| IT-E31005LIC-OO | 600V/100A/0.5m*2pcs Ring terminal low inductance |
| IT-E31010LIC-OO | 600V/100A/1m*2pcs Ring terminal low inductance |
| IT-E31020LIC-OO | 600V/100A/2m*2pcs Ring terminal low inductance |
| IT-E31040LIC-OO | 600V/100A/2m*2pcs Ring terminal low inductance |
| IT-E31220-OO | 500V/120A/2m*2pcs Ring terminals-Ring terminals |
| IT-E31250-OO | 500V/120A/5m*2pcs Ring terminals-Ring terminals |
| IT-E32410-OO | 500V/240A/1m*2pcs Ring terminals-Ring terminals |
| IT-E32420-OO | 500V/240A/2m*2pcs Ring terminals-Ring terminals |
| IT-E32450-OO | 500V/240A/5m*2pcs Ring terminals-Ring terminals |
| IT-E3301020-OO | 3kV/100A/2m*2pcs Ring terminals-Ring terminals |
| IT-E3301050-OO | 3kV/100A/5m*2pcs Ring terminals-Ring terminals |
| IT-E3302420-OO | 3kV/240A/2m*2pcs Ring terminals-Ring terminals |
| IT-E3302450-OO | 3kV/240A/5m*2pcs Ring terminals-Ring terminals |
| IT-E3303620-OO | 3kV/360A/2m*2pcs Ring terminals-Ring terminals |
| IT-E3304020-OO | 3kV/400A/2m*2pcs Ring terminals-Ring terminals |
| IT-E33620-OO | 500V/360A/2m*2pcs Ring terminals-Ring terminals |
| IT-E33650-OO | 500V/360A/5m*2pcs Ring terminals-Ring terminals |
| IT-E34020-OO | 500V/400A/2m*2pcs Ring terminals-Ring terminals |
| IT-E34520-OO | 500V/450A/2m*2pcs Ring terminals-Ring terminals |
| IT-E35030-OO | 500V/360A/3m*2pcs Ring terminals-Ring terminals |
| IT-E36530-OO | 500V/650A/3m*2pcs Ring terminals-Ring terminals |

For maximum current of AWG copper wire, refer to table below.

| AWG | 10 | 12 | 14 | 16 | 18 | 20 | 22 | 24 | 26 | 28 |
|-------------------------------|----|----|----|----|----|----|----|-----|-----|-----|
| The Maximum current value(A) | 40 | 25 | 20 | 13 | 10 | 7 | 5 | 3.5 | 2.5 | 1.7 |

Note: AWG (American Wire Gage), it means X wire (marked on the wire). The table above lists current capacity of single wire at working temperature of 30°C. For reference only.



Connect with us

Thank you for purchasing ITECH products. Any questions, pls. feel free to let us know.



You can chat with us on ITECH website



For more information, pls. visit www.itechate.com



Click and follow ITECH Electronics

